

Technical Publications

1694829

Revision 3

OEC Elite MiniView Software Release Workstation 1.x DICOM CONFORMANCE STATEMENT

Copyright© 2015 by General Electric Co.

Do not duplicate



GE Healthcare

REVISION HISTORY

REV	DATE	REASON FOR CHANGE
1	Dec 17 2014	Initial Release
2	Oct 15 2015	Update document per Support Center Review Comments: DCS_Review_Rev1.xls Change Bits Stored from 14 to 12 for Table 4-8, Table 4-10 and Section 10.4.1. Change High Bit from 13 to 11 for Table 4-8, Table 4-10 and Section 10.4.1. Change Requested Procedure Code Sequence from Empty to Not send for Acquisition without MWL Entry for Table 7-3.
3	Nov 05 2015	Update document per Support Center Review Comments: Update copyright date from 2014 to 2015.

THIS PAGE LEFT INTENTIONALLY BLANK

CONFORMANCE STATEMENT OVERVIEW

This DICOM Conformance Statement captures the DICOM capabilities of the OEC Elite MiniView identified below.

Table 0.1 provides an overview of the network services supported by OEC Elite MiniView system.

Table 0.1 – NETWORK SERVICES

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Transfer		
Computed Radiography Image Storage	No	Yes
Secondary Capture Image Storage	No	Yes
X-Ray Angiographic Image Storage	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	No	Yes
X-Ray Radiation Dose SR	Yes	No
Query/Retrieve		
Patient Root Query/Retrieve Information Model – FIND	Yes	No
Patient Root Query/Retrieve Information Model – MOVE	Yes	No
Study Root Query/Retrieve Information Model – FIND	Yes	No
Study Root Query/Retrieve Information Model – MOVE	Yes	No
Print Management		
Basic Film Session SOP Class	Yes	No
Basic Film Box SOP Class	Yes	No
Basic Grayscale Image Box SOP Class	Yes	No
Basic Grayscale Print Management Meta SOP Class	Yes	No
Printer SOP Class	Yes	No
Workflow Management		
Storage Commitment Push Model SOP Class	Yes	No
Modality Performed Procedure Step SOP Class	Yes	No
Modality Worklist Information Model – FIND SOP Class	Yes	No

Table 0.2 provides an overview of the Media Storage Application Profiles supported by OEC Elite MiniView system.

Table 0.2 - MEDIA SERVICES

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
Compact Disk - Recordable		
General Purpose CD-R	Yes	Yes

TABLE OF CONTENTS

1.	INTRODUCTION	11
1.1	Overview	11
1.2	Overall DICOM Conformance Statement Document Structure.....	12
1.3	Intended Audience	13
1.4	Scope and Field of Application	13
1.5	Important Remarks	13
1.6	References.....	14
1.7	Definitions.....	14
1.8	Symbols and Abbreviations.....	16
2.	NETWORK CONFORMANCE STATEMENT	19
2.1	Introduction.....	19
2.2	Implementation Model.....	19
2.2.1	Application Data Flow Diagram	19
2.2.2	Functional Definition of AE's.....	21
2.2.3	Sequencing of Real-World Activities.....	22
2.3	AE Specifications	22
2.3.1	Workstation AE Specification.....	22
2.3.1.1	Association Establishment Policies	23
2.3.1.1.1	General.....	23
2.3.1.1.2	Number of Associations.....	23
2.3.1.1.3	Asynchronous Nature.....	23
2.3.1.1.4	Implementation Identifying Information	23
2.3.1.2	Association Initiation Policy	24
2.3.1.2.1	Real-World Activity “Storage”	24
2.3.1.2.1.1	Associated Real-World Activity	24
2.3.1.2.1.2	Proposed Presentation Context Table	24
2.3.1.2.1.2.1	SOP Specific DICOM Conformance Statement for All Storage SOP Classes.....	24
2.3.1.2.1.2.2	SOP Specific DICOM Conformance Statement for the X-Ray Radiation Dose Storage SOP Classes	25
2.3.1.2.1.2.3	SOP Specific DICOM Conformance Statement for the Storage Commitment Push Model SOP Class SCU	25
2.3.1.2.2	Real-World Activity “DICOM Print”	26
2.3.1.2.2.1	Associated Real-World Activity	26
2.3.1.2.2.2	Proposed Presentation Context Table	26
2.3.1.2.2.2.1	SOP Specific DICOM Conformance Statement for Basic Grayscale Print Management SOP Classes	27
2.3.1.2.2.2.1.1	Basic Film Session SOP Class	28

2.3.1.2.2.2.1.2	Basic Film Box SOP Class.....	29
2.3.1.2.2.2.1.3	Basic Grayscale Image Box SOP Class	32
2.3.1.2.2.2.1.4	Printer SOP Class.....	33
2.3.1.2.3	Real-World Activity “Verify”	34
2.3.1.2.3.1	Associated Real-World Activity	34
2.3.1.2.3.2	Proposed Presentation Context Table	34
2.3.1.2.3.2.1	SOP Specific DICOM Conformance Statement for Verify SOP Classes.....	34
2.3.1.2.4	Real-World Activity “Modality Worklist Query”	35
2.3.1.2.4.1	Associated Real-World Activity	35
2.3.1.2.4.2	Proposed Presentation Context Table	35
2.3.1.2.4.2.1	SOP Specific DICOM Conformance Statement for the Modality Worklist Information Model - FIND SOP Class	35
2.3.1.2.5	Real-World Activity “Report MPPS”	36
2.3.1.2.5.1	Associated Real-World Activity	36
2.3.1.2.5.2	Proposed Presentation Context Table	36
2.3.1.2.5.2.1	SOP Specific DICOM Conformance Statement for Modality Performed Procedure Step SOP Class	36
2.3.1.2.6	Real-World Activity “Query/Retrieve”	37
2.3.1.2.6.1	Associated Real-World Activity	37
2.3.1.2.6.2	Proposed Presentation Context Table	38
2.3.1.2.6.2.1	SOP Specific DICOM Conformance Statement for the Patient Root Query/Retrieve Information Model - FIND, Study Root Query/Retrieve Information Model - FIND SOP Classes	38
2.3.1.2.6.2.2	SOP Specific DICOM Conformance Statement for the Patient Root Query/Retrieve Information Model - MOVE , Study Root Query/Retrieve Information Model - MOVE SOP Classes.....	39
2.3.1.3	Association Acceptance Policy	40
2.3.1.3.1	Real-World Activity “Local Store SCP”	40
2.3.1.3.1.1	Associated Real-World Activity	40
2.3.1.3.1.2	Accepted Presentation Context Table	40
2.3.1.3.1.2.1	SOP Specific DICOM Conformance Statement for all Storage SOP Classes	41
2.3.1.3.2	Real-World Activity “Verification SCP”	41
2.3.1.3.2.1	Associated Real-World Activity	41
2.3.1.3.2.2	Accepted Presentation Context Table	41
2.4	Communication Profiles	42
2.4.1	Supported Communication Stacks	42
2.4.2	Physical Media Support	42
2.4.3	Additional Protocol	42
2.4.4	IPv4 and IPv6 Support	42
2.5	Extensions / Specializations/ Privatizations	42
2.6	Configuration	42
2.6.1	AE Title/Presentation Address Mapping.....	42
2.6.2	Configurable Parameters	42
2.7	Support of Extended Character Sets.....	44
2.8	Codes and Controlled Terminology.....	44
2.9	Security Profiles	44
3.	MEDIA STORAGE CONFORMANCE STATEMENT	45
3.1	Introduction.....	45
3.1.1	Application Data Flow Diagram	45

3.1.2	Functional Definition of AE's	45
3.1.3	Sequencing of Real-World Activities.....	46
3.1.4	File Meta Information Options (See PS3.10).....	46
3.2	AE Specifications	46
3.2.1	Workstation AE Specification.....	46
3.2.1.1	File Meta Information for the Workstation Application Entity.....	46
3.2.1.2	Real-World Activities for the Workstation Application Entity	47
3.2.1.2.1	Real-World Activity Storage	47
3.2.1.2.1.1	Media Storage Application Profile for the RWA Update File Set	47
3.2.1.2.1.1.1	Options for STD-GEN-CD Application Profile.....	47
3.2.2	Media Viewer AE Specification	47
3.2.2.1	File Meta Information for the Media Viewer Application Entity	48
3.2.2.2	Real-World Activities for the Media Viewer Application Entity	48
3.2.2.2.1	Real-World Activity Directory Listing	48
3.2.2.2.1.1	Media Storage Application Profile for the RWA Directory Listing	48
3.2.2.2.1.1.1	STD-GEN-CD Application Profile.....	48
3.2.3	Media Viewer AE Specification	49
3.3	Augmented and Private Application Profiles	49
3.4	Extensions / Specializations / Privatizations	49
3.5	Configuration	49
3.6	Support of Extended Character Sets.....	49
4.	X-RAY ANGIOGRAPHIC INFORMATION OBJECT IMPLEMENTATION	50
4.1	Introduction.....	50
4.2	OEC Elite MiniView Mapping of DICOM Entities	50
4.3	IOD Module Table	50
4.4	Information Module Definitions	51
4.4.1	Patient Entity Modules.....	52
4.4.1.1	Patient Module	52
4.4.2	Study Entity Modules.....	53
4.4.2.1	General Study Module	53
4.4.3	Series Entity Modules	54
4.4.3.1	General Series Module.....	54
4.4.4	Equipment Entity Modules.....	56
4.4.4.1	General Equipment Module	56
4.4.5	Image Entity Modules	56
4.4.5.1	General Image Module.....	56
4.4.5.2	Image Pixel Module	57
4.4.5.3	Contrast/Bolus Module	58
4.4.5.4	X-Ray Image Module.....	59
4.4.5.4.1	Image Type	60
4.4.5.5	X-Ray Acquisition Module	60
4.4.5.6	XA Positioner Module	61
4.4.5.7	Overlay Plane Module.....	61
4.4.5.8	VOI LUT module.....	62
4.4.5.9	SOP Common Module	62

4.5	Standard Extended and Private Data Attributes	66
4.5.1	Standard Attributes	66
4.6	Standard Extended and Private Context Groups	66
5.	X-RAY RADIATION DOSE STRUCTURED REPORT INFORMATION OBJECT IMPLEMENTATION	67
5.1	Introduction.....	67
5.2	OEC Elite MiniView Mapping of DICOM Entities	67
5.3	IOD Module Table	67
5.4	Information Module Definitions	68
5.4.1	Patient Entity Modules.....	68
5.4.1.1	Patient Module	68
5.4.2	Study Entity Modules.....	70
5.4.2.1	General Study Module	70
5.4.2.2	Patient Study Module	70
5.4.3	Series Entity Modules	71
5.4.3.1	SR Document Series Module	71
5.4.4	Equipment Entity Modules.....	72
5.4.4.1	General Equipment Module	72
5.4.5	Document Entity Modules	72
5.4.5.1	SR Document General Module	72
5.4.5.2	SR Document Content Module	74
5.4.5.2.1	SR Document Content Descriptions	74
5.4.5.2.1.1	Content Template.....	74
5.4.5.3	SOP Common Module	75
5.5	Standard Extended and Private Data Attributes	77
5.6	Standard Extended and Private Context Groups	77
5.6.1	Standard Extended Context Groups	77
5.6.2	Configurable Context Groups	77
5.7	Standard, Standard Extended and Private Templates	77
5.7.1	Standard Templates.....	77
5.7.1.1	Template ID 10001 X-Ray Radiation Dose	78
5.7.1.2	Template ID 10002 Accumulated X-Ray Dose.....	79
5.7.1.3	Template ID 10003 Irradiation Event X-Ray Data	80
5.7.1.4	Template ID 10004 Accumulated Projection X-Ray Dose	84
5.7.1.5	Template ID 1002 Observer Context	85
5.7.1.6	Template ID 1004 Device Observer Identifying Attributes	86
5.7.2	Standard Extended Templates.....	86
6.	MODALITY WORKLIST QUERY IMPLEMENTATION	87
6.1	Introduction.....	87
6.2	OEC Elite MiniView Mapping of DICOM Entities	87
6.3	Worklist Query Module Table.....	87

6.4	Worklist Query Module Definitions	88
6.4.1	Common Scheduled Procedure Step Entity Modules.....	88
6.4.1.1	SOP Common Module	88
6.4.1.1.1	Specific Character Set.....	88
6.4.1.2	Scheduled Procedure Step Module	89
6.4.1.2.1	Scheduled Station AE Title.....	91
6.4.2	Common Requested Procedure Entity Modules.....	91
6.4.2.1	Requested Procedure Module	91
6.4.2.1.1	Study Instance UID.....	92
6.4.3	Common Imaging Service Request Entity Modules.....	93
6.4.3.1	Imaging Service Request Module	93
6.4.4	Common visit Entity Modules.....	94
6.4.4.1	Visit Identification	94
6.4.4.2	Visit Status	94
6.4.4.3	Visit Relationship.....	94
6.4.4.4	Visit Admission.....	94
6.4.5	Common Patient Entity Modules	94
6.4.5.1	Patient Relationship	94
6.4.5.2	Patient Identification	94
6.4.5.3	Patient Demographic	95
6.4.5.4	Patient Medical	96
7.	MODALITY PERFORMED PROCEDURE STEP IMPLEMENTATION	97
7.1	Introduction.....	97
7.2	Relationship between Scheduled and Performed Procedure Steps	97
7.3	Modality Performed Procedure Step Module Table.....	97
7.4	Modality Performed Procedure Step Module Definitions.....	97
7.4.1	SOP Common Module	98
7.4.2	Performed Procedure Step Relationship Module	98
7.4.3	Performed Procedure Step Information Module	100
7.4.4	Image Acquisition Results Module	101
7.4.5	Radiation Dose Module	102
7.4.6	Billing and Material Management Codes Module	103
7.5	Standard Extended and Private Data Attributes	103
7.5.1	Standard Attributes	103
7.6	Standard Extended and Private Context Groups	103
7.6.1	Standard Extended Context Groups	103
7.6.1.1	Context ID 9301 Modality PPS Discontinuation Reasons	104
8.	STORAGE COMMITMENT PUSH MODEL IMPLEMENTATION.....	105
8.1	Storage Commitment Push Model Information Object Definition.....	105
8.1.1	STORAGE COMMITMENT MODULE FOR N-ACTION.....	105
8.1.2	STORAGE COMMITMENT MODULE FOR N-EVENT-REPORT	105
8.1.2.1	Processing of Failure Reason when received in a N-Event-Report	106
9.	BASIC DIRECTORY INFORMATION OBJECT IMPLEMENTATION	107

9.1	IOD Module Table	107
9.2	Information Module Definitions	107
9.2.1	File Set identification Module.....	108
9.2.2	Directory Information Module	108
9.2.3	Definition of Specific Directory Records.....	109
9.2.3.1	Patient Directory Record Definition.....	109
9.2.3.2	Study Directory Record Definition	109
9.2.3.3	Series Directory Record Definition	110
9.2.3.3.1	Icon Image Key Definition	110
9.2.3.4	Image Directory Record Definition.....	111
9.2.3.4.1	Icon Image Key Definition	111
9.2.3.5	SR Document Directory Record Definition	112
9.3	Private Data Dictionary.....	112
10.	PRINT MANAGEMENT IMPLEMENTATION.....	113
10.1	Introduction.....	113
10.2	Basic Film Session SOP Class	113
10.2.1	Basic Film Session N-Create Attributes.....	113
10.2.2	Basic Film Session N-Delete.....	113
10.3	Basic Film Box SOP Class	113
10.3.1	Basic Film Box N-Create Attributes	113
10.3.2	Basic Film Box N-Action Attributes.....	115
10.3.3	Basic Film Box N-Delete	115
10.4	Basic Grayscale Image Box SOP Class	115
10.4.1	Basic Grayscale Image Box Pixel N-Set Attributes	115
10.5	Printer SOP Class	116
10.5.1	Printer N-Event-Report Attributes	116
10.5.2	Printer N-Get Attributes	117
11.	QUERY IMPLEMENTATION.....	118
11.1	OEC Elite MiniView Mapping of DICOM Entities	118
11.2	Information Model Keys	118
11.2.1	Common Query Keys.....	118
11.2.1.1	Q/R Common Attribute Descriptions	119
11.2.1.1.1	Specific Character Set.....	119
11.2.2	Patient Level	119
11.2.3	Study Level – Patient Root	120
11.2.4	Study Level – Study Root	121
11.2.5	Series Level.....	123
11.2.6	Image Level.....	124

1. INTRODUCTION

1.1 OVERVIEW

This DICOM Conformance Statement is divided into Sections as described below:

Section 1 (Introduction), which describes the overall structure, intent, and references for this Conformance Statement

Section 2 (Network Conformance Statement), which specifies the GEHC equipment compliance to the DICOM requirements for the implementation of Networking features.

Section 3 (Media Storage Conformance Statement), specifies the OEC Elite MiniView equipment compliance to the DICOM requirements for the implementation of Media Storage features.

Section 4 (X-Ray Angiographic Information Object Implementations), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of an X-Ray Information Objects.

Section 5 (X-Ray Radiation Dose SR Information Object Implementations), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of X-Ray Radiation Dose SR Information Object Implementation feature.

Section 6 (Modality Worklist Query Information Model), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of the Modality Worklist service.

Section 7 (Modality Performed Procedure Step Implementation), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of the Modality Performed Procedure Step SOP Classes.

Section 8 (Storage Commitment Push Model Implementation), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of the Storage Commitment Push feature.


Section 9 (Basic Directory Information Object Implementation), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of a Basic Directory Information Object.

Section 10 (Print Management Implementation), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of the Basic Print Meta SOP Classes (Grayscale).

Section 11 (Query/Retrieve Information Model), specifies the OEC Elite MiniView Medical Systems equipment compliance to DICOM requirements for the implementation of the Patient, Study Root Query/Retrieve service.

1.2 OVERALL DICOM CONFORMANCE STATEMENT DOCUMENT STRUCTURE

The Documentation Structure of the GEHC DICOM Conformance Statements is shown in the Illustration below.

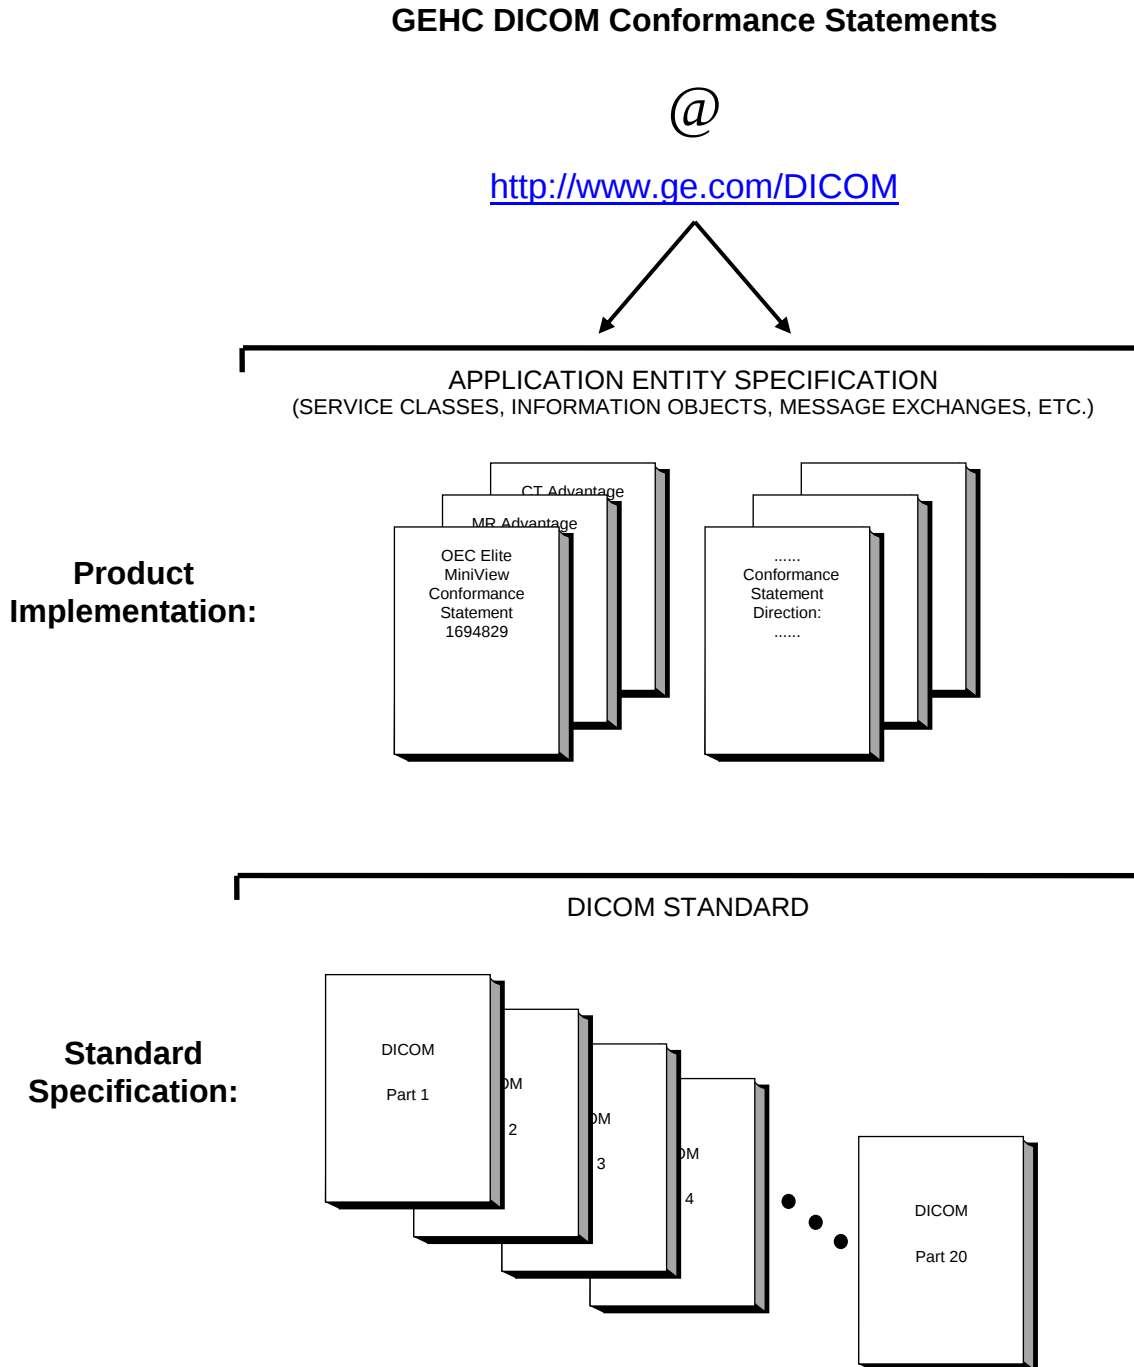

This document specifies the DICOM implementation. It is entitled:

OEC Elite MiniView Version Workstation-1.x
Conformance Statement for DICOM
1694829

This DICOM Conformance Statement documents the DICOM Conformance Statement and Technical Specification required interoperating with the GEHC network interface.

The GEHC Conformance Statement, contained in this document, also specifies the Lower Layer communications which it supports (e.g., TCP/IP). However, the Technical Specifications are defined in the DICOM Part 8 standard.

For more information regarding DICOM, copies of the Standard may be obtained on the Internet at <http://medical.nema.org>. Comments on the Standard may be addressed to:

DICOM Secretariat
NEMA
1300 N. 17th Street, Suite 1752
Rosslyn, VA 22209
USA
Phone: +1.703.841.3200

1.3 INTENDED AUDIENCE

The reader of this document is concerned with software design and/or system integration issues. It is assumed that the reader of this document is familiar with the DICOM Standard and with the terminology and concepts which are used in that Standard.

1.4 SCOPE AND FIELD OF APPLICATION

It is the intent of this document to provide an unambiguous specification for GEHC implementations. This specification, called a Conformance Statement, includes a DICOM Conformance Statement and is necessary to ensure proper processing and interpretation of GEHC medical data exchanged using DICOM. The GEHC Conformance Statements are available to the public.

The reader of this DICOM Conformance Statement should be aware that different GEHC devices are capable of using different Information Object Definitions. For example, a GEHC CT Scanner may send images using the CT Information Object, MR Information Object, Secondary Capture Object, etc.

Included in this DICOM Conformance Statement are the Module Definitions which define all data elements used by this GEHC implementation. If the user encounters unspecified private data elements while parsing a GEHC Data Set, the user is well advised to ignore those data elements (per the DICOM standard). Unspecified private data element information is subject to change without notice. If, however, the device is acting as a "full fidelity storage device", it should retain and re-transmit all of the private data elements which are sent by GEHC devices.

1.5 IMPORTANT REMARKS

The use of these DICOM Conformance Statements, in conjunction with the DICOM Standards, is intended to facilitate communication with GE imaging equipment. However,

by itself, it is not sufficient to ensure that inter-operation will be successful. The **user (or user's agent)** needs to proceed with caution and address at least four issues:

- **Integration** - The integration of any device into an overall system of interconnected devices goes beyond the scope of standards (DICOM v3.0), and of this introduction and associated DICOM Conformance Statements when interoperability with non-GE equipment is desired. The responsibility to analyze the applications requirements and to design a solution that integrates GE imaging equipment with non-GE systems is the **user's** responsibility and should not be underestimated. The **user** is strongly advised to ensure that such an integration analysis is correctly performed.
- **Validation** - Testing the complete range of possible interactions between any GE device and non-GE devices, before the connection is declared operational, should not be overlooked. Therefore, the **user** should ensure that any non-GE provider accepts full responsibility for all validation required for their connection with GE devices. This includes the accuracy of the image data once it has crossed the interface between the GE imaging equipment and the non-GE device and the stability of the image data for the intended applications.

Such a validation is required before any clinical use (diagnosis and/or treatment) is performed. It applies when images acquired on GE imaging equipment are processed/displayed on a non-GE device, as well as when images acquired on non-GE equipment is processed/displayed on a GE console or workstation.

- **Future Evolution** - GE understands that the DICOM Standard will evolve to meet the user's growing requirements. GE is actively involved in the development of the DICOM Standard. DICOM will incorporate new features and technologies and GE may follow the evolution of the Standard. The GEHC protocol is based on DICOM as specified in each DICOM Conformance Statement. Evolution of the Standard may require changes to devices which have implemented DICOM. **In addition, GE reserves the right to discontinue or make changes to the support of communications features (on its products) described by these DICOM Conformance Statements.** The **user** should ensure that any non-GE provider, which connects with GE devices, also plans for the future evolution of the DICOM Standard. Failure to do so will likely result in the loss of function and/or connectivity as the DICOM Standard changes and GE Products are enhanced to support these changes.
- **Interaction** - It is the sole responsibility of the **non-GE provider** to ensure that communication with the interfaced equipment does not cause degradation of GE imaging equipment performance and/or function.

1.6 REFERENCES

NEMA PS3	Digital Imaging and Communications in Medicine (DICOM) Standard, available free at http://medical.nema.org/
----------	--

1.7 DEFINITIONS

Informal definitions are provided for the following terms used in this Conformance Statement. The DICOM Standard is the authoritative source for formal definitions of these terms.

Abstract Syntax – the information agreed to be exchanged between applications, generally equivalent to a Service/Object Pair (SOP) Class. Examples: Verification SOP Class, Modality Worklist Information Model Find SOP Class, Computed Radiography Image Storage SOP Class.

Application Entity (AE) – an end point of a DICOM information exchange, including the DICOM network or media interface software; i.e., the software that sends or receives DICOM information objects or messages. A single device may have multiple Application Entities.

Application Entity Title – the externally known name of an *Application Entity*, used to identify a DICOM application to other DICOM applications on the network.

Application Context – the specification of the type of communication used between *Application Entities*. Example: DICOM network protocol.

Association – a network communication channel set up between *Application Entities*.

Attribute – a unit of information in an object definition; a data element identified by a *tag*. The information may be a complex data structure (Sequence), itself composed of lower level data elements. Examples: Patient ID (0010,0020), Accession Number (0008,0050), Photometric Interpretation (0028,0004), Procedure Code Sequence (0008,1032).

Information Object Definition (IOD) – the specified set of *Attributes* that comprise a type of data object; does not represent a specific instance of the data object, but rather a class of similar data objects that have the same properties. The *Attributes* may be specified as Mandatory (Type 1), Required but possibly unknown (Type 2), or Optional (Type 3), and there may be conditions associated with the use of an Attribute (Types 1C and 2C). Examples: MR Image IOD, CT Image IOD, Print Job IOD.

Joint Photographic Experts Group (JPEG) – a set of standardized image compression techniques, available for use by DICOM applications.

Media Application Profile – the specification of DICOM information objects and encoding exchanged on removable media (e.g., CDs)

Module – a set of *Attributes* within an *Information Object Definition* that are logically related to each other. Example: Patient Module includes Patient Name, Patient ID, Patient Birth Date, and Patient Sex.

Negotiation – first phase of *Association* establishment that allows *Application Entities* to agree on the types of data to be exchanged and how that data will be encoded.

Presentation Context – the set of DICOM network services used over an *Association*, as negotiated between *Application Entities*; includes *Abstract Syntaxes* and *Transfer Syntaxes*.

Protocol Data Unit (PDU) – a packet (piece) of a DICOM message sent across the network. Devices must specify the maximum size packet they can receive for DICOM messages.

Security Profile – a set of mechanisms, such as encryption, user authentication, or digital signatures, used by an *Application Entity* to ensure confidentiality, integrity, and/or availability of exchanged DICOM data

Service Class Provider (SCP) – role of an *Application Entity* that provides a DICOM network service; typically, a server that performs operations requested by another *Application Entity* (*Service Class User*). Examples: Picture Archiving and Communication System (image storage SCP, and image query/retrieve SCP), Radiology Information System (modality worklist SCP).

Service Class User (SCU) – role of an *Application Entity* that uses a DICOM network service; typically, a client. Examples: imaging modality (image storage SCU, and modality worklist SCU), imaging workstation (image query/retrieve SCU)

Service/Object Pair (SOP) Class – the specification of the network or media transfer (service) of a particular type of data (object); the fundamental unit of DICOM interoperability specification. Examples: Ultrasound Image Storage Service, Basic Grayscale Print Management.

Service/Object Pair (SOP) Instance – an information object; a specific occurrence of information exchanged in a *SOP Class*. Examples: a specific x-ray image.

Tag – a 32-bit identifier for a data element, represented as a pair of four digit hexadecimal numbers, the “group” and the “element”. If the “group” number is odd, the tag is for a private (manufacturer-specific) data element. Examples: (0010,0020) [Patient ID], (07FE,0010) [Pixel Data], (0019,0210) [private data element]

Transfer Syntax – the encoding used for exchange of DICOM information objects and messages. Examples: *JPEG* compressed (images), little endian explicit value representation.

Unique Identifier (UID) – a globally unique “dotted decimal” string that identifies a specific object or a class of objects; an ISO-8824 Object Identifier. Examples: Study Instance UID, SOP Class UID, SOP Instance UID.

Value Representation (VR) – the format type of an individual DICOM data element, such as text, an integer, a person’s name, or a code. DICOM information objects can be transmitted with either explicit identification of the type of each data element (Explicit VR), or without explicit identification (Implicit VR); with Implicit VR, the receiving application must use a DICOM data dictionary to look up the format of each data element.

1.8 SYMBOLS AND ABBREVIATIONS

AE	Application Entity
AET	Application Entity Title
Workstation	OEC Elite MiniView Workstation
Workstation AE	OEC Elite MiniView Workstation AE
CAD	Computer Aided Detection
CD-R	Compact Disk Recordable
CR	Computed Radiography
CT	Computed Tomography
DB	Database
DHCP	Dynamic Host Configuration Protocol
DICOM	Digital Imaging and Communications in Medicine

DX	Digital X-ray
FSC	File-Set Creator
FSU	File-Set Updater
FSR	File-Set Reader
HL7	Health Level 7 Standard
HLF	High Level Fluoro
IOD	Information Object Definition
IPv4	Internet Protocol version 4
IPv6	Internet Protocol version 6
ISO	International Organization for Standards
JPEG	Joint Photographic Experts Group
LUT	Look-up Table
MPPS	Modality Performed Procedure Step
MR	Magnetic Resonance Imaging
MWL	Modality Worklist
O	Optional (Key Attribute)
PACS	Picture Archiving and Communication System
PDU	Protocol Data Unit
R	Required (Key Attribute)
RDSR	Radiation Dose Structured Reports
RF	Radiofluoroscopy
SC	Secondary Capture
SCP	Service Class Provider
SCU	Service Class User
SOP	Service-Object Pair
SPS	Scheduled Procedure Step
SR	Structured Reporting
TCP/IP	Transmission Control Protocol/Internet Protocol

GE Healthcare
1694829 REV 3

U	Unique (Key Attribute)
VR	Value Representation
XA	X-ray Angiography

2. NETWORK CONFORMANCE STATEMENT

2.1 INTRODUCTION

This section of the DICOM Conformance Statement specifies the OEC Elite MiniView compliance to DICOM requirements for **Networking** features.

OEC Elite MiniView runs on industrial computer. It provides the following DICOM functionalities:


- Send Echo message to DICOM Verification SCP.
- Export DICOM images and RDSR to a DICOM Storage SCP.
- Query DICOM Modality Worklist from a DICOM Worklist SCP.
- Querying for saved examinations and retrieving saved examinations from a DICOM Query/Retrieve SCP
- Sending exam start and end messages to a DICOM Modality Performed Procedure Step SCP.
- Sending storage commitment requests to a DICOM Storage Commitment SCP.
- Print acquired images to a DICOM Printer.

2.2 IMPLEMENTATION MODEL

2.2.1 Application Data Flow Diagram

The network application model for the OEC Elite MiniView is shown in the following Illustration :

ILLUSTRATION 2-1
OEC ELITE MINIVIEW NETWORK APPLICATION MODEL AND DATA FLOW DIAGRAM

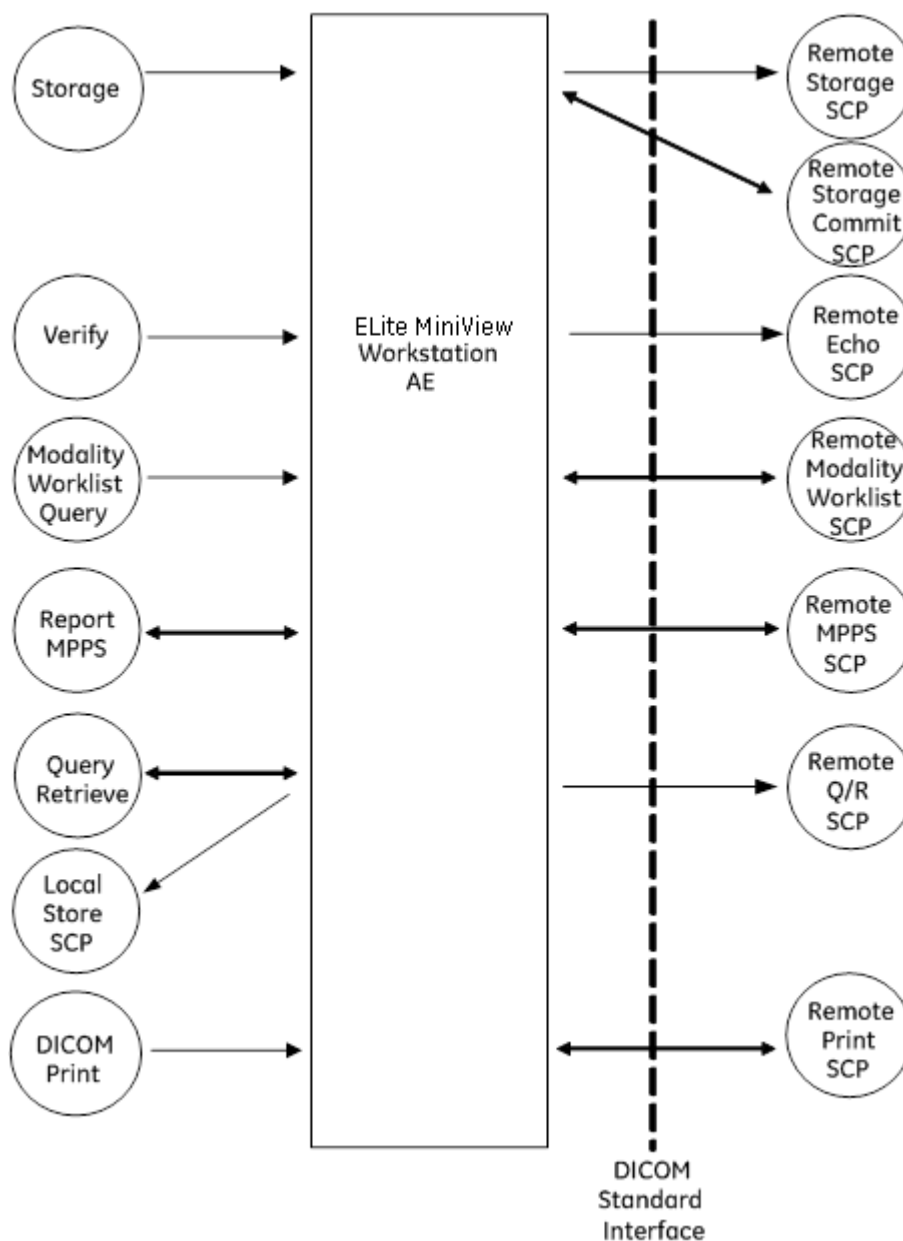

The product supports activity “Storage” which performs images/RDSR storage and storage commitment functions; The results of that functionalities are communicated to Remote Store Server for DICOM image/RDSR storage and storage commitment.

The product supports activity “Print” which performs images print functions; The results of that functionalities are communicated to Remote Printer/Server for DICOM image print functions.

The product supports activity “Verify” which interacts with Remote Verify SCP for DICOM Echo purpose.

The product supports activity “Modality Worklist Query” which performs Modality worklist query, from remote Modality Worklist SCP.

The product supports activity “Query”: Initiate an association with a Remote AE to query for images on the remote host. Once the association has been established, it sends a sequence of requests (Patient, then Study then Series Level requests) to the Remote AE. After all responses are received, Workstation AE will issue a Series-Level C-FIND-RQ request to get the series for a study in the list.

The product supports activity “Retrieve”: Send a C-MOVE-RQ request to a Remote AE after successful association establishment. The Workstation AE’s Storage SCP will receive the images over a separate association.

The product supports activity “Report MPPS”: When the user begins the image acquisition process and generates the first image, the Workstation AE sends N-CREATE message to the configured MPPS SCP to indicate that the image acquisition process has been started for the requested procedure. The operator can close the acquisition session either by completing the acquisition process or discontinuing the ongoing scan. On closing the acquisition session, the Workstation AE sends N-SET message to the configured MPPS SCP to indicate the acquisition state of the requested procedure, with appropriate MPPS status (COMPLETED/DISCONTINUED).

2.2.2 Functional Definition of AE's

Application Entity “OEC Elite MiniView Workstation AE (i.e. Workstation AE)” initiates the following functionalities :

- DICOM Host Verification: Initiate an association and send a C-ECHO-RQ message to the remote DICOM AE; the remote DICOM server will send back a C-ECHO-RSP message with a status of “success” if the operation is successful.
- DICOM Image Storage: Initiate an association to a remote AE to send image(s). If the remote AE accept the presentation context applicable to the image(s), the WorkstationAE will send the image(s) by invoking C-STORE-RQ operation for each image on the same association. The remote DICOM server will send back C-STORE-RSP with status “success” if the operation is successful.
- Storage Commitment: Initiates a DICOM Storage Commitment request once a Store request has completed successfully. An N-ACTION request specifying all the successfully transferred images will be issued to the remote AE. The remote AE will reply accepting or refusing the request on the same association. If accepted the remote AE will issue an N-EVENT response specifying which images have been committed and which, if any, have not.
- Modality Worklist Query: Initiate an association with a remote AE to query for scheduled exams, a C-FIND-RQ request will be sent to the remote AE. C-FIND-RSP with query results will be received.
- Query: Initiate an association with a Remote AE to query for images on the remote host. Follows the Patient->Study->Series sequence C-FIND-RQ request (the request more than once) will be sent to the Remote AE once an association has been established. Once all the responses have been received, the operator needs to select an exam in the local database browser; on selection of the exam the DICOM Server AE will issue a Series-Level C-FIND-RQ request to get the series for a study in the list. Similarly the Image-Level C-FIND-RQ will be issued for the series selected from the series list.

- Retrieve: Send a C-MOVE-RQ request to a Remote AE for retrieve of images after successful establishment. At this time the Local Store SCP listener will start, not until after receiving complete images the Local Store SCP listener will stopped.
- DICOM Print: Initiate an association with a remote AE to print grayscale images, please refer to Section 2.3.1.2.2.1 for details.

2.2.3 Sequencing of Real-World Activities

This sequence is only applicable for Remote AE where Storage Commitment Option is allowed in Network Manager.

1. The user selects the images and sends them to a remote host.

2. If the remote DICOM AE is associated with a Storage Commitment Provider AE and if the images are successfully sent to the DICOM AE, then an N-ACTION-RQ request is sent automatically to the associated Storage Commitment Provider AE. The Storage Commitment Provider AE can be configured independently from the remote DICOM AE with network address, port and AE title.

2.3 AE SPECIFICATIONS

2.3.1 Workstation AE Specification

The Workstation Application Entity provides Standard Conformance to the following DICOM SOP Classes as an SCU and/or as an SCP:

SOP Class Name	SOP Class UID	SCU	SCP
Verification SOP Class	1.2.840.10008.1.1	Yes	No
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	No	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	No	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	No	Yes
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Yes	No
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	No
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	No
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	No
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Yes	No
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Yes	No
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No

Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Yes	No
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Yes	No
Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No

2.3.1.1 Association Establishment Policies

2.3.1.1.1 General

The DICOM Application Context Name (ACN), which is always proposed, is:

Application Context Name	1.2.840.10008.3.1.1.1
---------------------------------	------------------------------

The maximum length PDU receive size for the Workstation AE is:

Maximum Length PDU	16384
---------------------------	--------------

2.3.1.1.2 Number of Associations

The Workstation AE will initiate a maximum of 1 simultaneous association to remote nodes.

The Workstation AE will support a maximum of 1 simultaneous associations initiated by remote nodes.

2.3.1.1.3 Asynchronous Nature

Asynchronous mode is not supported. All operations will be performed synchronously.

2.3.1.1.4 Implementation Identifying Information

The Implementation UID for this DICOM Implementation is:

OEC Elite MiniView Implementation UID	1.2.840.113619.6.403
OEC Elite MiniView Implementation Version Name	GEHC_OEC_101

2.3.1.2 Association Initiation Policy

When the Workstation Application Entity initiates an Association for any Real-World Activity, it will propose the Presentation Contexts for all Real-World Activities; i.e., there is only a single, comprehensive Presentation Context Negotiation proposed for the AE.

The Workstation AE proposes only a single Transfer Syntax in each Presentation Context; i.e., for each Abstract Syntax in the following Presentation Context Tables, the AE proposes one Presentation Context for each specified Transfer Syntax.

2.3.1.2.1 Real-World Activity “Storage”

2.3.1.2.1.1 Associated Real-World Activity

Upon a request by the operator the selected images will be sent to the configured DICOM Store SCP.

2.3.1.2.1.2 Proposed Presentation Context Table

Presentation Context Table – Proposed by Workstation AE for Activity Storage				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name List	UID List	
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU

2.3.1.2.1.2.1 SOP Specific DICOM Conformance Statement for All Storage SOP Classes

The Workstation AE includes optional data elements in the SOP Instances as described in Sections 4.

Although the Modality Type could be configured to “RF/XA/CR/SC” when user export image to interchange media or remote DICOM server, only XA Image IOD is used.

Following are the status codes that are more specifically processed when receiving messages from a **Storage** SCP equipment : If store command completed normally, with a status of success or some warning then the image was accepted.

Service Status	Status Code	Further Meaning	Application Behavior When Receiving Status Code
Failure	A700-A7FF	Refused: Out of resources	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays store failure message.
	A900-A9FF	Error: Data Set does not match SOP Class	
	C000-CFFF	Error: Cannot Understand	
	0122	SOP Class Not Supported	
Warning	B000	Coercion of Data Elements	Ignored by application and current operation continues
	B006	Elements Discarded	
	B007	Data Set does not match SOP Class	
Success	0000	DICOM storage operation is success	The DICOM operation progress screen disappearance indicates current operation is success.
*	*	Any other status code.	Upon receiving a C-STORE confirmation containing a Refused status, this implementation will terminate the association.

2.3.1.2.1.2.2 SOP Specific DICOM Conformance Statement for the X-Ray Radiation Dose Storage SOP Classes

See Section 2.3.1.2.1.2.1 “SOP Specific DICOM Conformance Statement for All Storage SOP Classes” for details on general Storage Service SCU processing also applicable to the X-Ray Radiation Dose Storage SOP Classes.

The Workstation AE supports creation and transmission of X-Ray Radiation Dose SOP Instances referencing Instances of the following Storage SOP Classes:

SOP Class Name	SOP Class UID
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67

2.3.1.2.1.2.3 SOP Specific DICOM Conformance Statement for the Storage Commitment Push Model SOP Class SCU

The Workstation AE uses DICOM network storage services to transfer SOP Instances which are to be committed.

The Workstation AE may request Storage Commitment for Instances of any of the Composite SOP Classes it supports as an SCU (see Section 2.3.1.2.1.2.1).

The Storage Commitment Information Object is described in Section 8.

Upon receiving a Storage Commitment N-EVENT-REPORT (Storage Commitment Result on the same association), the Workstation AE will return a Success status.

Note: N-EVENT-REPORT is only expected on the same association.

Following are the status codes that are more specifically processed when receiving N-Action responses from Storage Commitment SCP equipment:

Service Status	Status Code	Further Meaning	Application Behavior When Receiving Status Code
Failure	0119	Class-instance conflict	Terminates the association and operation. Logs failure message along with error comment returned from SCP and displays failure message.
	0210	Duplicate invocation	
	0115	Invalid argument value	
	0117	Invalid SOP Instance	
	0212	Mistyped argument	
	0123	No such action	
	0114	No such argument	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Success	0000		The progress screen is disappeared.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.2 Real-World Activity “DICOM Print”

2.3.1.2.2.1 Associated Real-World Activity

Upon a request by the operator the selected images will be sent to the configured DICOM Printer (DICOM Print SCP).

2.3.1.2.2.2 Proposed Presentation Context Table

Presentation Context Table – Proposed by AE Workstation for Activity DICOM Print					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

2.3.1.2.2.1 SOP Specific DICOM Conformance Statement for Basic Grayscale Print Management SOP Classes

The Workstation AE uses the following DIMSE services of the supported SOP Classes:

SOP Class	SOP Class UID	DIMSE Service Element	SCU Usage
Basic Film Session	1.2.840.10008.5.1.1.1	N-CREATE	Used (Mandatory)
		N-SET	Not Used
		N-DELETE	Used
		N-ACTION	Not Used
Basic Film Box	1.2.840.10008.5.1.1.2	N-CREATE	Used (Mandatory)
		N-ACTION	Used (Mandatory)
		N-DELETE	Used
		N-SET	Not Used
Printer	1.2.840.10008.5.1.1.16	N-EVENT-REPORT	Used (Mandatory)
		N-GET	Used
Basic Grayscale Image Box	1.2.840.10008.5.1.1.4	N-SET	Used (Mandatory)

When a manual print operation is initiated, the AE:

1. Initiates a DICOM association and negotiates Presentation Contexts
2. N-GETs printer status using the Printer SOP Class
3. N-CREATEs a Basic Film Session SOP Instance, and then followed by N-DELETE of the Basic Film Session SOP Instance.
4. N-CREATEs a Basic Film Box SOP Instance for each film
5. N-SETs the Image Box SOP Instance for each image on the film
6. Prints by N-ACTION on the Basic Film Box SOP Instances, then followed by N-DELETE of the Basic Film Box SOP Instance
7. Receives N-EVENT-REPORTs of the well know Printer SOP Instance indicating printer status if the SCP send a request.

8. Releases the DICOM association after printing is successful or failure has been signaled to the user

9. The DICOM operation progress screen disappearance indicates current operation is success.

The Print management IODs is defined in Section.

2.3.1.2.2.1.1 Basic Film Session SOP Class

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Basic Film Session SOP Class N-CREATE:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	0119	Class-instance conflict	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	0210	Duplicate invocation	
	0111	Duplicate SOP Instance	
	0106	Invalid attribute value	
	0117	Invalid SOP instance	
	0120	Missing attribute	
	0121	Missing attribute value	
	0212	Mistyped argument	
	0105	No such attributes	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Warning	B600	Memory allocation not supported	Ignored by application and current operation continues
Success	0000	Film session successfully created	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Basic Film Session SOP Class N-DELETE:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	0119	Class-instance conflict	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	0210	Duplicate invocation	
	0117	Invalid SOP instance	
	0212	Mistyped argument	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Success	0000	Film session successfully deleted	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.2.1.2 Basic Film Box SOP Class

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Basic Film Box SOP Class N-CREATE:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	C616	There is an existing Film Box that has not been printed and N-ACTION at the Film Session level is not supported. A new Film Box will not be created when a previous Film Box has not been printed.	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	0119	Class-instance conflict	
	0210	Duplicate invocation	
	0111	Duplicate SOP Instance	
	0106	Invalid attribute value	

Warning	0117	Invalid SOP instance	
	0120	Missing attribute	
	0121	Missing attribute value	
	0212	Mistyped argument	
	0105	No such attributes	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
	B605	Requested Min Density or Max Density outside of printer's operating range. The printer will use its respective minimum or maximum density value instead.	Ignored by application and current operation continues.
Success	0000	Film box successfully created	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Basic Film Box SOP Class N-ACTION:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	C602	Unable to create Print Job SOP Instance; print queue is full	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	C603	Image size is larger than image box size (by using the specified magnification value)	
	C604	Image position collision : multiple images assigned to single image position	
	C613	Combined Print Image size is larger than the Image Box size	
	0119	Class-instance conflict	
	0210	Duplicate invocation	
	0115	Invalid argument value	
	0117	Invalid SOP Instance	
	0212	Mistyped argument	

	0123	No such action	
	0114	No such argument	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Warning	B603	Film Box SOP Instance hierarchy does not contain Image Box SOP Instances (empty page)	Ignored by application and current operation continues.
	B604	Image size is larger than image box size, the image has been demagnified.	
	B609	Image size is larger than the Image Box size. The Image has been cropped to fit.	
	B60A	Image size or Combined Print Image size is larger than the Image Box size. Image or Combined Print Image has been decimated to fit.	
Success	0000	Film accepted for printing; if supported, the Print Job SOP Instance is created	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Basic Film Box SOP Class N-DELETE:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	0119	Class-instance conflict	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	0210	Duplicate invocation	
	0117	Invalid SOP instance	
	0212	Mistyped argument	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	

Success	0000	Film box successfully deleted	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.2.1.3 Basic Grayscale Image Box SOP Class

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Basic Grayscale Image Box SOP Class N-SET:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	C603	Image size is larger than image box size	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	C605	Insufficient memory in printer to store the image	
	C613	Combined Print Image size is larger than the Image Box size	
	0119	Class-instance conflict	
	0210	Duplicate invocation	
	0106	Invalid attribute value	
	0212	Mistyped argument	
	0117	Invalid SOP instance	
	0121	Missing attribute value	
	0105	No such attributes	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Warning	B604	Image size larger than image box size, the image has been demagnified.	Ignored by application and current operation continues.
	B605	Requested Min Density or Max Density outside of printer's operating range. The printer will use its respective minimum	

		or maximum density value instead.	
	B609	Image size is larger than the Image Box size. The Image has been cropped to fit.	
	B60A	Image size or Combined Print Image size is larger than the Image Box size. The Image or Combined Print Image has been decimated to fit.	
Success	0000	Image successfully stored in Image Box	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.2.1.4 Printer SOP Class

The Workstation AE supports the Printer SOP Class to receive information on the status of the printer.

For the product behavior description when receiving N-Event-Report request, refer to section 10.5.1 Printer N-Event-Report Attributes.

Also, following are the status codes the Application may send back in the **N-Event-Report** response command to the **Printer SOP Class** SCP Equipment that sent the N-Event-Report request:

Service Status	Status Code	Further Meaning	Status Code Explanation	Related Fields Sent Back to the SCP
Success	0000		If an N-EVENT-REPORT DIMSE service is received when the association is active, Print SCU handles the relevant states but the data received is ignored and send back "Success".	None

For the attribute list requested by this product and for the behavior of this product on each returned value, refer to Section 10.5.22 Printer N-Get Attributes

Following are the status codes that are more specifically processed when receiving messages from a **Print** SCP equipment for the Printer SOP Class N-GET:

Service Status	Status Codes	Further Meaning	Application Behavior When receiving Status Codes
Failure	0107	Attribute list error	Terminate the operation. Logs store failed message along with error comment returned from SCP. Displays print failure message.
	0119	Class-instance conflict	
	0210	Duplicate invocation	

	0117	Invalid SOP instance	
	0212	Mistyped argument	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Success	0000	Success	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.3 Real-World Activity “Verify”

2.3.1.2.3.1 Associated Real-World Activity

The user may initiate a DICOM Verify Request in the configuration screen for each respective remote SCP configuration (Print, Store, Worklist Query, MPPS, SC and Q/R).

A valid response from the SCP will result in a “The DICOM server has verified successfully” screen displayed on the screen. In the event that the SCP does not response for some reason, the operation will timeout and the Workstation AE will close the association and results in “The DICOM Verify Fails” screen displayed to user.

Note: The default timeout is 30 seconds for DICOM Echo and this value could be configured from system setup screen.

2.3.1.2.3.2 Proposed Presentation Context Table

Presentation Context Table – Proposed by Workstation AE for Activity Verify					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

2.3.1.2.3.2.1 SOP Specific DICOM Conformance Statement for Verify SOP Classes

The message “The DICOM server has verified successfully” is displayed when the DICOM Verify is successfully performed, otherwise message “The DICOM Verify Fails” is displayed.

2.3.1.2.4 Real-World Activity “Modality Worklist Query”

2.3.1.2.4.1 Associated Real-World Activity

Upon a request by the operator, the current scheduled exam list should be updated from the remote Modality Worklist Server.

2.3.1.2.4.2 Proposed Presentation Context Table

Presentation Context Table – Proposed by Workstation AE for Activity Modality Worklist				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name List	UID List	
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
		Explicit VR Little Endian	1.2.840.10008.1.2.1	
		Explicit VR Big Endian	1.2.840.10008.1.2.2	

2.3.1.2.4.2.1 SOP Specific DICOM Conformance Statement for the Modality Worklist Information Model - FIND SOP Class

The Workstation AE includes matching keys in the Modality Worklist queries as described in Section 6.

The results of the Worklist query are displayed to the user in the Scheduled Exam Screen. Currently, the maximal capability of received scheduled exams is 500 and not configurable.

The Workstation AE checks the Specific Character Set tag (0008,0005) contained in a C-FIND RSP, ISO_IR 100 or blank will be accepted, and all other value will be discarded. Responses without this tag will also be accepted.

A C-FIND CANCEL will be sent when the maximal capability of received scheduled exams(500 exams) is reached or user cancels operation by clicking the Cancel button on the progressing screen.

Following are the status codes that are more specifically processed when receiving messages from a **Modality Worklist** SCP equipment:

Service Status	Status Code	Further Meaning	Application Behavior When Receiving Status Code
Failure	A700	Refused: Out of resources	Terminates the association and operation. Logs failure message along with error comment returned from SCP and displays failure message.
	A900	Error: Identifier does not match SOP Class	
	C000-CFFF	Error: Unable to process	
	0122	SOP Class Not Supported	

GE Healthcare
1694829 REV 3

Cancel	FE00	Matching terminated due to cancel	The progress screen is disappeared, the received scheduled exams will be displayed.
Success	0000	Matching is complete - No final identifier is supplied	The progress screen is disappeared, all the received scheduled exams will be displayed.
Pending	FF00	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys.	The progress screen is still displayed.
	FF01	Matches are continuing - Warning that one or more Optional Keys were not supported for existence for this Identifier	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.5 Real-World Activity “Report MPPS”

2.3.1.2.5.1 Associated Real-World Activity

The Modality Performed Procedure Step N-CREATE is sent with status of “IN PROGRESS” when start exam is initiated by the operator. The Modality Performed Procedure Step N-SET is sent with status of “COMPLETED” when the exam is completed (all images acquired). If the exam is aborted, a status of “DISCONTINUED” is sent.

2.3.1.2.5.2 Proposed Presentation Context Table

Presentation Context Table – Proposed by OEC Elite MiniView AE for Activity Modality Worklist					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

2.3.1.2.5.2.1 SOP Specific DICOM Conformance Statement for Modality Performed Procedure Step SOP Class

MPPS will be created at the start of an image acquisition step; an MPPS will be set after the completion/discontinue of a post-processing step when the user selects “Complete”/“Discontinue”.

The Workstation AE includes attributes in the Modality Performed Procedure Step N-CREATE as described in Section 7.4

Following are the status codes that are more specifically processed when receiving an N-Create or N-Set response from an **MPPS** SCP equipment:

Service Status	Status Code	Further Meaning	Application Behavior When Receiving Status Code
Failure	0119	Class-instance conflict	Terminates the association and operation. Logs failure message along with error comment returned from SCP and displays failure message.
	0210	Duplicate invocation	
	0106	Invalid attribute value	
	0117	Invalid SOP instance	
	0120	Missing attribute	
	0121	Missing attribute value	
	0212	Mistyped argument	
	0105	No such attributes	
	0118	No such SOP Class	
	0112	No such SOP Instance	
	0110	Processing failure	
	0213	Resource limitation	
	0211	Unrecognized operation	
Success	0000		The progress screen is disappeared.
	0111	Duplicate SOP Instance	
*	*	Any other status code.	Deemed a failure.

2.3.1.2.6 Real-World Activity “Query/Retrieve”

2.3.1.2.6.1 Associated Real-World Activity

Upon a request from the user, a C-FIND-RQ command will be issued to the Query/Retrieve SCP to query for exams that match the user-defined query criteria. The association will be released upon the receipt of the C-FIND-RSP confirmation. To retrieve an exam, the user can either use the information returned from a query or the information stored in the local database when the exam was archived. The C-MOVE-RQ command is used to retrieve the exam from the Query/Retrieve SCP. The C-STORE-RQ from the SCP is expected on another association.

After a DICOM file is retrieved, the attributes are extracted and saved onto the local system.

2.3.1.2.6.2 Proposed Presentation Context Table

Presentation Context Table – Proposed by OEC Elite MiniView AE for Activity Modality Worklist				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name List	UID List	
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU

2.3.1.2.6.2.1 SOP Specific DICOM Conformance Statement for the Patient Root Query/Retrieve Information Model - FIND, Study Root Query/Retrieve Information Model - FIND SOP Classes

The Workstation AE includes matching keys in the queries as described in Sections 11.

The Acquisition AE evaluates a C-FIND RSP containing the Specific Character Set tag (0008,0005). Values of ISO_IR 100 or blank will be accepted, and all others will be rejected.

Responses without this tag will also be accepted.

A C-FIND CANCEL will be sent when the display limit for results is reached.

The product does not support Extended Negotiation for C-FIND.

Following are the status codes that are more specifically processed when receiving messages from a Query SCP equipment:

Service Status	Status Code	Further Meaning	Application Behavior When Receiving Status Code
Failure	A700	Refused: Out of resources	Terminates the association and operation. Logs failure message along with error comment returned from SCP and displays failure message.
	A900	Error: Identifier does not match	

GE Healthcare
1694829 REV 3

		SOP Class	
	C000-CFFF	Error: Unable to process	
	0122	SOP Class Not Supported	
Cancel	FE00	Matching terminated due to cancel	The progress screen is disappeared, the received scheduled exams will be displayed
Success	0000	Matching is complete - No final identifier is supplied	The progress screen is disappeared, all the received scheduled exams will be displayed.
Pending	FF00	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys.	The progress screen is still displayed.
	FF01	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this Identifier	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.2.6.2.2 SOP Specific DICOM Conformance Statement for the Patient Root Query/Retrieve Information Model - MOVE , Study Root Query/Retrieve Information Model - MOVE SOP Classes

The C-MOVE-RQ will use the AE Title of the Workstation Application Entity as the Move Destination AE Title.

A C-FIND CANCEL message is sent if the user clicks the Cancel button during the move.

Following are the status codes that are more specifically processed when receiving messages from a **Retrieve** SCP equipment:

Service Status	Status Code	Further Meaning	Application Behavior When Receiving Status Code
Failure	A701	Refused: Out of resources - Unable to calculate number of matches	Terminates the association and operation. Logs failure message along with error comment returned from SCP and displays failure message.
	A702	Refused: Out of resources - Unable to perform sub-operations	
	A801	Refused: Move Destination Unknown	

GE Healthcare
1694829 REV 3

	A900	Error: Identifier does not match SOP Class	
	C000-CFFF	Error: Unable to process	
	0122	SOP Class Not Supported	
Cancel	FE00	Sub-operations terminated due to a Cancel indication	The progress screen is disappeared, the received scheduled exams will be displayed
Warning	B000	Sub-operations Complete - One or more Failures.	Ignored by application and current operation continues.
Success	0000	Sub-operations Complete - No Failure.	The progress screen is disappeared, all the received scheduled exams will be displayed.
Pending	FF00	Sub-operations are continuing -	The progress screen is still displayed.
*	*	Any other status code.	Deemed a failure.

2.3.1.3 Association Acceptance Policy

If the Remote AE needs to “Query/Retrieve Images”, to the local system then it has to be configured in the Local system to do the same.

When the DICOM Server AE accepts an association for image storage, it will receive any images transmitted on that association and store the images on disk.

It will also respond to queries from Remote AEs by sending matching entries. Any Remote AE can request and receive a list of images on the local database. The Remote AE must be configured in the local config file list of Remote AE for it to be able to retrieve images from DICOM Server AE.

2.3.1.3.1 Real-World Activity “Local Store SCP”

2.3.1.3.1.1 Associated Real-World Activity

The Real-World Activity associated with the Receive Images operation is the storage of the image on the disk drive.

2.3.1.3.1.2 Accepted Presentation Context Table

Presentation Context Table - Accepted by AE Workstation for Activity Receive Images					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
X-Ray	1.2.840.10008.5.1.4.	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Angiographic Image Storage	1.1.12.1	Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2		
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

2.3.1.3.1.2.1 SOP Specific DICOM Conformance Statement for all Storage SOP Classes

The Workstation AE provides Level 2 (FULL) Conformance, and stores all standard and private data elements of received SOP Instances.

Following are the status codes the Application may send back to the SCU Equipment after performing the requested **Storage**:

Service Status	Status Code	Further Meaning	Status Code Explanation	Related Fields Sent Back to the SCU
Failure	A700	Refused: Out of resources	Out of Disk space	(0000,0902)
Success	0000			None

2.3.1.3.2 Real-World Activity “Verification SCP”

2.3.1.3.2.1 Associated Real-World Activity

An incoming Verification request will cause the Workstation AE to accept the association and respond with a verification response after the Retrieve DICOM Server AE accepts an sub-association for image storage.

2.3.1.3.2.2 Accepted Presentation Context Table

Presentation Context Table - Accepted by AE Workstation for Activity Receive Images					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification SOP Class	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

2.4 COMMUNICATION PROFILES

2.4.1 Supported Communication Stacks

The DICOM Upper Layer Protocol is supported using TCP/IP, as specified in DICOM PS3.8.

The TCP/IP stack is inherited from the Linux Operating System.

2.4.2 Physical Media Support

The product is provided with a 10/100 Mb/s or 1Gb/s auto-sensing Ethernet interface. Additional or alternate network interfaces may be available.

2.4.3 Additional Protocol

The Workstation supports DHCP, user could configure DHCP Enable/Disable from System Setup screen. When DHCP is Enabled, then, the network information will be gotten automatically.

Default is Enabled.

2.4.4 IPv4 and IPv6 Support

The Workstation only supports IPv4.

2.5 EXTENSIONS / SPECIALIZATIONS/ PRIVATIZATIONS

Not Applicable.

2.6 CONFIGURATION

2.6.1 AE Title/Presentation Address Mapping

2.6.2 Configurable Parameters

The following fields are configurable:

The default value for these fields is blank unless otherwise specified.

Network

- Use DHCP or static IP (Default –DHCP).
- Local IP Address
- Local Subnet mask
- Default Gateway

Configuration:

- Local AE Title (Default – GEHC OEC)

- Station Name
- Hospital Name

Every Remote DICOM AE SCP: (Store, Storage Commitment, MPPS, Print, Modality Worklist, Query/Retrieve)

- Server Alias
- Remote AE Title
- Remote IP Address
- Remote Port Number
- Gateway IP Address.
- Modality Type (Default - RF)

Additional fields for Remote DICOM Print

- Min Density for Printer
- Max Density for Printer
- Configuration Information
- Border Density
- Empty Density
- Number of Copies
- Print Priority
- Film Destination
- Medium Type
- Film Size
- Format
- Film Orientation

Additional fields for Remote DICOM Query Worklist Filter

- Patient Name
- Patient ID
- Requested Procedure ID
- Accession Number
- Exam Date: Today, Next 2 Days, Next 3 Days, Next 7 Days, Date Range
- Performing Physician Name
- Modality Type (Default - RF)

Additional fields for Remote DICOM Query/Retrieve Filter

- Date: Today, Next 2 Days, Next 3 Days...
- Patient Name
- Patient ID
- Accession Number
- Modality Type (Default - RF)

Note: All configurations must be performed by a GE Field Engineer.

2.7 SUPPORT OF EXTENDED CHARACTER SETS

As a Query SCU, it will similarly accept response items with ISO_IR 100 values of Specific Character Set or empty value of Specific Character Set (absence of (0008,0005) which mean usage of ASCII Chars only).

The product user interface will allow the user to enter characters from the console keyboard that is within ISO 8859-1. Responses with non-compatible values of (0008,0005) will be discarded.

2.8 CODES AND CONTROLLED TERMINOLOGY

The product uses no coded terminology.

2.9 SECURITY PROFILES

The product does not conform to any defined DICOM Security Profiles.

It is assumed that the product is used within a secured environment. It is assumed that a secured environment includes at a minimum:

1. Firewall or router protections to ensure that only approved external hosts have network access to the product.
2. Firewall or router protections to ensure that the product only has network access to approved external hosts and services.
3. Any communications with external hosts and services outside the locally secured environment use appropriate secure network channels (such as a Virtual Private Network (VPN))

3. MEDIA STORAGE CONFORMANCE STATEMENT

3.1 INTRODUCTION


This section of the DICOM conformance statement specifies the Workstation AE compliance to DICOM requirements for **Media Interchange**. It details the DICOM Media Storage Application Profiles and roles that are supported by this product.

The Workstation AE is able to export images and RDSR to DICOM media.

3.1.1 Application Data Flow Diagram

The media interchange application model for the Workstation AE is shown in the following Illustration:

ILLUSTRATION 3-1
WORKSTATION AE MEDIA INTERCHANGE APPLICATION MODEL AND DATA FLOW DIAGRAM

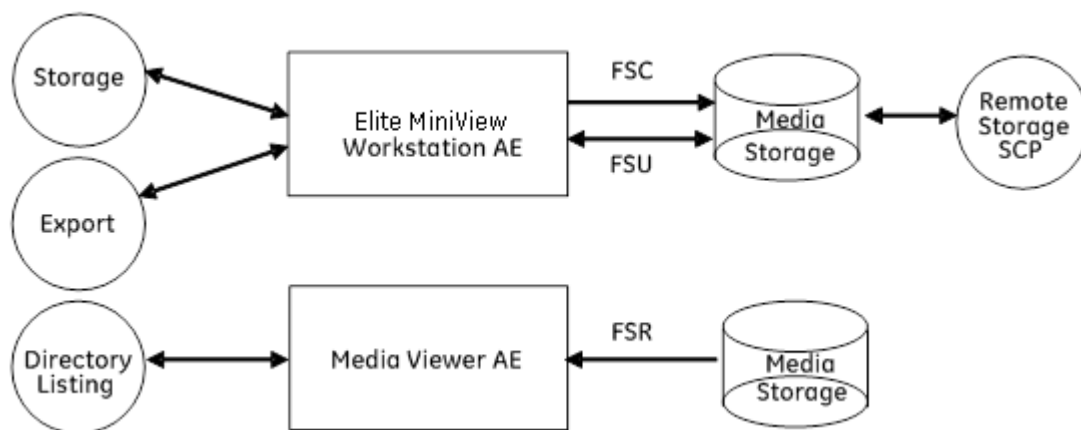

The Workstation AE supports the General Purpose CD-R Interchange profiles.

3.1.2 Functional Definition of AE's

The Workstation AE can perform these functions:

- Create a new DICOM File-Set on Media
- Update a DICOM File-Set by adding new SOP instances to the media which supports multi-session.

The Media Viewer AE can perform this function:

- Reads a DICOM File-Set from media and reviews recorded DICOM instances (including images and RDSR).

3.1.3 Sequencing of Real-World Activities

Storage/Export – Images are acquired and archived on OEC Elite MiniView; From the Image Directory screen, images/RDSR can be selected and copied to media; Images/RDSR can be viewed by any DICOM application that supports Media Exchange FSR and X-Ray Radiation Dose Structured Reports.

Directory Listing – During the Image Copy, user could choice copying image/RDSR with a Media Viewer, then the images/RDSR will be copied with a Media Viewer instance; Images/RDSR can be viewed by this media viewer only on Windows OS (Independent of the OEC Elite MiniView Workstation AE).

3.1.4 File Meta Information Options (See PS3.10)

The File Meta-Information for this implementation is:

File Meta-Information Version	1
OEC Elite MiniView Implementation UID	1.2.840.113619.6.403
OEC Elite MiniView Implementation Version Name	GEHC_OEC_101

3.2 AE SPECIFICATIONS

3.2.1 Workstation AE Specification

The Workstation Application Entity provides standard conformance to DICOM Interchange Option of the Media Storage Service Class. The supported Application Profiles and roles are listed below.

Supported Application Profile	Real World Activity	Role	Option
STD-GEN-CD	Storage/ Export	FSC,FSU	Interchange

3.2.1.1 File Meta Information for the Workstation Application Entity

Following are the values set in the File Meta Information for this AE Title:

Source Application Entity Title	Not used
OEC Elite MiniView Implementation UID	1.2.840.113619.6.403
OEC Elite MiniView Implementation Version Name	GEHC_OEC_101

3.2.1.2 Real-World Activities for the Workstation Application Entity

3.2.1.2.1 Real-World Activity Storage

The Workstation AE acts as a FSC/FSU when requested to copy SOP instance from local database to the interchange media.

When user selects “Storage” function, the selected images should be saved as DICOM SOP instances and copied to media. The DICOM File set on the media should be created or updated accordingly.

3.2.1.2.1.1 Media Storage Application Profile for the RWA Update File Set

For the list of Application Profiles that invoke this AE for the Real-World Activity Storage, see the Table in Section 3.2.1 “OEC Elite MiniView” where the table describing the Application Profiles and Real-World Activity is defined.

3.2.1.2.1.1.1 Options for STD-GEN-CD Application Profile

Following are the optional SOP Classes supported by this AE. All SOP Instances use the Explicit VR Little Endian Uncompressed Transfer Syntax, UID 1.2.840.10008.1.2.1.

SOP Class	SOP Class UID
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1

Common DICOMDIR Directory Records created by this AE will include key attributes as described in Section 9. Following are the Additional DICOMDIR Keys supported for this profile:

ADDITIONAL DICOMDIR KEYS

Key Attribute	Tag	Directory Record Type	Type	Notes
Image Type	(0008,0008)	IMAGE	1C	FSC/FSU: Present when the DICOMDIR file is created and this value should be extracted from referenced image file.

3.2.2 Media Viewer AE Specification

The Media Viewer Application Entity provides standard conformance to DICOM Interchange of the Media Storage Service Class. The supported Application Profiles and roles are listed below.

Supported Application Profile	Real World Activity	Role
STD-GEN-CD	Directory Listing	FSR

3.2.2.1 File Meta Information for the Media Viewer Application Entity

Following are the values set in the File Meta Information for this AE Title:

Source Application Entity Title	Not used
Media Viewer Implementation UID	Not used
Implementation Version Name	Not used

Since Media Viewer just used to read file-set and display image, so, above information could not be set by Media Viewer.

3.2.2.2 Real-World Activities for the Media Viewer Application Entity

3.2.2.2.1 Real-World Activity Directory Listing

The Media Viewer AE acts as a FSR when listing the directory information from interchange media.

When user load the media on Window OS, the Media Viewer will read the DICOM File-Set and display/list the DICOM directory entries for those instances in the File-Set on the media.

3.2.2.2.1.1 Media Storage Application Profile for the RWA Directory Listing

For the list of Application Profiles that invoke this AE for the Real-World Activity Directory Listing, see the Table in Section 3.2.3 “Media Viewer AE Specification” where the table describing the Application Profiles and Real-World Activity is defined.

3.2.2.2.1.1.1 STD-GEN-CD Application Profile

Following are the SOP Classes supported by this AE and only the Explicit VR Little Endian Uncompressed Transfer Syntax (UID 1.2.840.10008.1.2.1) is supported.

SOP Class	SOP Class UID
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1

Common DICOMDIR Directory Records read by this AE will include key attributes as described in Section 9. Following are the Additional DICOMDIR Keys supported for this profile:

Key Attribute	Tag	Directory Record Type	Type	Notes
Image Type	(0008,0008)	IMAGE	1C	FSR: Used.

3.2.3 Media Viewer AE Specification

The Media Viewer Application Entity provides standard conformance to DICOM Interchange of the Media Storage Service Class. The supported Application Profiles and roles are listed below.

Supported Application Profile	Real World Activity	Role
STD-GEN-CD	Directory Listing	FSR

3.3 AUGMENTED AND PRIVATE APPLICATION PROFILES

No augmented/private profile is implemented.

3.4 EXTENSIONS / SPECIALIZATIONS / PRIVATIZATIONS

No Extensions / Specializations / Privatizations are implemented.

3.5 CONFIGURATION

CD Options (Media Exchange)

- Modality Type (Image Default – RF, Dose Summary Default – SC)
- Remove Patient Information (Default - No).
- Include Viewer (Default - Include)
- Include Overlay(Default - Include)

3.6 SUPPORT OF EXTENDED CHARACTER SETS

The Workstation AE will support fully only the ISO_IR 100 as extended character sets for media storage.

4. X-RAY ANGIOGRAPHIC INFORMATION OBJECT IMPLEMENTATION

4.1 INTRODUCTION

This section specifies the use of the DICOM X-Ray Angiographic Image IOD to represent the information included in X-Ray Angiographic Images by this implementation. Corresponding attributes are conveyed using the module construct.

4.2 OEC ELITE MINIVIEW MAPPING OF DICOM ENTITIES

The OEC Elite MiniView maps DICOM Information Entities to local Information Entities in the product's database and user interface.

TABLE 4-1
MAPPING OF DICOM ENTITIES TO OEC ELITE MINIVIEW ENTITIES

DICOM IE	OEC Elite MiniView Entity
Patient	Patient
Study	Exam
Series	Series
Equipment	Equipment
Image	Image

4.3 IOD MODULE TABLE

The X-Ray Angiographic Image Information Object Definition comprises the modules of the following table, plus Standard Extended and Private attributes. Standard Extended and Private attributes are described in Section 4.5.

TABLE 4-2
X-RAY ANGIOGRAPHIC IMAGE IOD MODULES

Entity Name	Module Name	Usage	Reference
Patient	Patient	Used	4.4.1.1
	Clinical Trial Subject	Not Used	N/A
Study	General Study	Used	4.4.2.1
	Patient Study	Not Used	N/A
	Clinical Trial Study	Not Used	N/A
Series	General Series	Used	4.4.3.1
	Clinical Trial Series	Not Used	N/A
Frame of Reference	Synchronization	Not Used	N/A

Equipment	General Equipment	Used	4.4.4.1
Image	General Image	Used	4.4.5.1
	Image Pixel	Used	4.4.5.2
	Contrast/Bolus	Used	4.4.5.3
	Cine	Not Used	N/A
	Multi-Frame	Not Used	N/A
	Frame Pointers	Not Used	N/A
	Mask	Not Used	N/A
	Display Shutter	Not Used	N/A
	Device	Not Used	N/A
	Intervention	Not Used	N/A
	X-Ray Image	Used	4.4.5.4
	X-Ray Acquisition	Used	4.4.5.5
	X-Ray Collimator	Not Used	N/A
	X-Ray Table	Not Used	N/A
	XA Positioner	Used	4.4.5.66
	DX Detector	Not Used	N/A
	Overlay Plane	Used	4.4.5.7
	Multi-Frame Overlay	Not Used	N/A
	Modality LUT	Not Used	N/A
	VOI LUT	Used	4.4.5.88
	SOP Common	Used	4.4.5.9
	Frame Extraction	Not Used	N/A

4.4 INFORMATION MODULE DEFINITIONS

Please refer to DICOM Part 3 (Information Object Definitions) for a description of each of the entities, modules, and attributes contained within the X-Ray Angiographic Information Object.

The following modules are included to convey Enumerated Values, Defined Terms, and Optional Attributes supported and/or expected. Type 1 & Type 2 Attributes are also included for completeness and to define what values they may take and where these values are obtained from when generating the instance as well as what are the expected values when loading such instance. It should be noted that they are the same ones as defined in the DICOM Standard Part 3 (Information Object Definitions). Also note that Attributes not present in tables are not supported.

GE Healthcare

1694829 REV 3

4.4.1 Patient Entity Modules

4.4.1.1 Patient Module

TABLE 4-3
PATIENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient's Name	(0010,0010)	2	May be entered from user interface or got from Worklist. Supports 5 different components delimited by “^”, 64 bytes maximum per component group.
Patient ID	(0010,0020)	2	May be entered from user interface or got from Worklist. Truncated to 64 bytes, end truncated.
Issuer of Patient ID	(0010,0021)	3	May be entered from user interface or got from Worklist. Truncated to 64 bytes, end truncated.
Patient's Birth Date	(0010,0030)	2	May be entered from user interface or got from Worklist Truncated to 8 bytes, end truncated
Patient's Sex	(0010,0040)	2	May be entered from user interface or got from Worklist. Truncated to 2 bytes, end truncated
Referenced Patient Sequence	(0008,1120)	3	Not Used
<i>>Include 'SOP Instance Reference Macro'</i>			
Patient's Birth Time	(0010,0032)	3	Not Used
Other Patient IDs	(0010,1000)	3	Not Used
Other Patient IDs Sequence	(0010,1002)	3	Not Used
>Patient ID	(0010,0020)	1	Not Used
>Issuer of Patient ID	(0010,0021)	1	Not Used
>Type of Patient ID	(0010,0022)	1	Not Used
Other Patient Names	(0010,1001)	3	Not Used
Ethnic Group	(0010,2160)	3	Not Used
Patient Comments	(0010,4000)	3	May be entered from user interface or got from Worklist From user interface truncated to 512 bytes. From worklist truncated to 10240 bytes.
Patient Species Description	(0010,2201)	1C	Not Used
Patient Species Code Sequence	(0010,2202)	1C	Not Used
<i>>Include 'Code Sequence Macro'</i>			
Patient Breed Description	(0010,2292)	2C	Not Used
Patient Breed Code Sequence	(0010,2293)	2C	Not Used
<i>>Include 'Code Sequence Macro'</i>			
Breed Registration Sequence	(0010,2294)	2C	Not Used

>Breed Registration Number	(0010,2295)	1	Not Used
>Breed Registry Code Sequence	(0010,2296)	1	Not Used
>>Include 'Code Sequence Macro'			
Responsible Person	(0010,2297)	2C	Not Used
Responsible Person Role	(0010,2298)	1C	Not Used
Responsible Organization	(0010,2299)	2C	Not Used
Patient Identity Removed	(0012,0062)	3	Used. If Patient Information is removed then set to "YES", otherwise set to "NO"
De-identification Method	(0012,0063)	1C	Used. If Patient Information is removed. Set to "Limited Data Set" in this case
De-identification Method Code Sequence	(0012,0064)	1C	Not Used
>Include 'Code Sequence Macro'			

4.4.2 Study Entity Modules

4.4.2.1 General Study Module

TABLE 4-4
GENERAL STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Study Instance UID	(0020,000D)	1	The product will adopt the Study Instance UID which is returned in the MWL response. If there is no Study Instance UID returned from MWL server, then new Study Instance UID will be created.
Study Date	(0008,0020)	2	This value is set to the exam created date.
Study Time	(0008,0030)	2	This value is set to the exam created time.
Referring Physician's Name	(0008,0090)	2	May be entered from the user interface or got from Worklist.
Referring Physician Identification Sequence	(0008,0096)	3	Not Used
>Include 'Person Identification Macro'			
Study ID	(0020,0010)	2	Generated by equipment.
Accession Number	(0008,0050)	2	May be entered from the user interface or got from Worklist.
Study Description	(0008,1030)	3	May be entered from the user interface or got from Worklist. The default value will be set as Requested Procedure Description when the tag got from MWL is not empty. Else this value will be set as Procedure Description on user interface.
Physician(s) of Record	(0008,1048)	3	Not Used

Physician(s) of Record Identification Sequence	(0008,1049)	3	Not Used
>Include 'Person Identification Macro'			
Name of Physician(s) Reading Study	(0008,1060)	3	Not Used
Physician(s) Reading Study Identification Sequence	(0008,1062)	3	Not Used
>Include 'Person Identification Macro'			
Referenced Study Sequence	(0008,1110)	3	Got from MWL.
>Include 'SOP Instance Reference Macro'			
Procedure Code Sequence	(0008,1032)	3	Not Used
>Include 'Code Sequence Macro'			

4.4.3 Series Entity Modules

4.4.3.1 General Series Module

TABLE 4-5
GENERAL SERIES MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Modality	(0008,0060)	1	This value could be set to RF/XA/CR/OT. The proper SOP class will be created based on XA Image IOD.
Series Instance UID	(0020,000E)	1	Created by equipment, using prefix: 1.2.840.113619.2.403. +MAC+seriesIndicator(20)+TimeStamp_Exam MAC: Number string of device MAC address.
Series Number	(0020,0011)	2	A number that identifies this Series.
Laterality	(0020,0060)	2C	The value is empty.
Series Date	(0008,0021)	3	This value is set to the first shot date.
Series Time	(0008,0031)	3	This value is set to the first shot time.
Performing Physicians' Name	(0008,1050)	3	Get from the Worklist scheduled performing physician, or the user can enter from the user interface.
Performing Physician Identification Sequence	(0008,1052)	3	Not Used
>Include 'Person Identification Macro'			
Protocol Name	(0018,1030)	3	When using MWL, if Scheduled Protocol Sequence Code Meaning is not empty then this value is Scheduled Protocol Sequence Code Meaning, else this value is Scheduled Procedure Step Description. It will be set as "Unknown Protocol" for local created exam.
Series Description	(0008,103E)	3	The value equal protocol Name.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

Operators' Name	(0008,1070)	3	Not Used
Operator Identification Sequence	(0008,1072)	3	Not Used
>Include 'Person Identification Macro'			
Referenced Performed Procedure Step Sequence	(0008,1111)	3	Used.
>Include 'SOP Instance Reference Macro'			
Related Series Sequence	(0008,1250)	3	Not Used
>Study Instance UID	(0020,000D)	1	Not Used
>Series Instance UID	(0020,000E)	1	Not Used
>Purpose of Reference Code Sequence	(0040,A170)	2	Not Used
>>Include 'Code Sequence Macro'			
Body Part Examined	(0018,0015)	3	Used
Patient Position	(0018,5100)	2C	Not Used
Smallest Pixel Value in Series	(0028,0108)	3	Not Used
Largest Pixel Value in Series	(0028,0109)	3	Not Used
Request Attributes Sequence	(0040,0275)	3	Used
>Requested Procedure ID	(0040,1001)	1C	Used
>Accession Number	(0008,0050)	3	Not Used
>Study Instance UID	(0020,000D)	3	Not Used
>Referenced Study Sequence	(0008,1110)	3	Not Used
>> Include 'SOP Instance Reference Macro'			
>Requested Procedure Description	(0032,1060)	3	Used
>Requested Procedure Code Sequence	(0032,1064)	3	Used
>>Include 'Code Sequence Macro'			
>Reason for the Requested Procedure	(0040,1002)	3	Not Used
>Reason for Requested Procedure Code Sequence	(0040,100A)	3	Not Used
>>Include 'Code Sequence Macro'			
>Scheduled Procedure Step ID	(0040,0009)	1C	Used
>Scheduled Procedure Step Description	(0040,0007)	3	Used
>Scheduled Protocol Code Sequence	(0040,0008)	3	Used
>>Include 'Code Sequence Macro'			
>>Protocol Context Sequence	(0040,0440)	3	Not Used
>>>Include 'Content Item Macro'			
>>>Content Item Modifier Sequence	(0040,0441)	3	Not Used
>>>>Include 'Content Item Macro'			
Performed Procedure Step ID	(0040,0253)	3	Used
Performed Procedure Step Start Date	(0040,0244)	3	Used
Performed Procedure Step Start Time	(0040,0245)	3	Used
Performed Procedure Step Description	(0040,0254)	3	Used

GE Healthcare
1694829 REV 3

Performed Protocol Code Sequence	(0040,0260)	3	Not Used
>Include 'Code Sequence Macro'			
>>Protocol Context Sequence	(0040,0440)	3	Not Used
>>>Include 'Content Item Macro'			
>>>Content Item Modifier Sequence	(0040,0441)	3	Not Used
>>>>Include 'Content Item Macro'			
Comments on the Performed Procedure Step	(0040,0280)	3	Not Used

4.4.4 Equipment Entity Modules

4.4.4.1 General Equipment Module

TABLE 4-6
GENERAL EQUIPMENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Manufacturer	(0008,0070)	2	This value is set to "GE Hualun Medical Systems, Co. Ltd".
Institution Name	(0008,0080)	3	Configurable by user on setup screen (The field name is "Hospital Name").
Institution Address	(0008,0081)	3	Not Used
Station Name	(0008,1010)	3	Configurable by user on DICOM setup screen.
Institutional Department Name	(0008,1040)	3	Not Used
Manufacturer's Model Name	(0008,1090)	3	This value is set to type and model of the system: "OEC Elite MiniView".
Device Serial Number	(0018,1000)	3	Configurable during system install.
Software Versions	(0018,1020)	3	This value is set to workstation software version.
Gantry ID	(0018,1008)	3	Not Used
Spatial Resolution	(0018,1050)	3	Not Used
Date of Last Calibration	(0018,1200)	3	Not Used
Time of Last Calibration	(0018,1201)	3	Not Used
Pixel Padding Value	(0028,0120)	1C	Not Used

4.4.5 Image Entity Modules

4.4.5.1 General Image Module

TABLE 4-7
GENERAL IMAGE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Instance Number	(0020,0013)	2	This value is set to image number.
Patient Orientation	(0020,0020)	2C	The value is empty.
Content Date	(0008,0023)	2C	This value is set to the date image was taken.

GE Healthcare
1694829 REV 3

Content Time	(0008,0033)	2C	This value is set to the time image was taken.
Image Type	(0008,0008)	3	See 4.4.5.4.1
Acquisition Number	(0020,0012)	3	This value is set to shot number.
Acquisition Date	(0008,0022)	3	Not Used
Acquisition Time	(0008,0032)	3	Not Used
Acquisition DateTime	(0008,002A))	3	This value is set to shot DateTime.
Referenced Image Sequence	(0008,1140)	3	Not Used
>Include 'SOP Instance Reference Macro'			
>Purpose of Reference Code Sequence	(0040,A170)	3	Not Used
>>Include 'Code Sequence Macro'			
Derivation Description	(0008,2111)	3	Not Used
Derivation Code Sequence	(0008,9215)	3	Not Used
>Include 'Code Sequence Macro'			
Source Image Sequence	(0008,2112)	3	Not Used
>Include 'SOP Instance Reference Macro'			
>Purpose of Reference Code Sequence	(0040,A170)	3	Not Used
>>Include 'Code Sequence Macro'			
>Spatial Locations Preserved	(0028,135A)	3	Not Used
>Patient Orientation	(0020,0020)	1C	Not Used
Referenced Instance Sequence	(0008,114A)	3	Not Used
>Include 'SOP Instance Reference Macro'			
>Purpose of Reference Code Sequence	(0040,A170)	1	Not Used
>>Include 'Code Sequence Macro'			
Images in Acquisition	(0020,1002)	3	Not Used
Image Comments	(0020,4000)	3	Not Used
Quality Control Image	(0028,0300)	3	Not Used
Burned In Annotation	(0028,0301)	3	Not Used
Lossy Image Compression	(0028,2110)	3	Not Used
Lossy Image Compression Ratio	(0028,2112)	3	Not Used
Lossy Image Compression Method	(0028,2114)	3	Not Used
Icon Image Sequence	(0088,0200)	3	Not Used
>Include 'Image Pixel Macro'			
Presentation LUT Shape	(2050,0020)	3	Not Used

4.4.5.2 Image Pixel Module

TABLE 4-8
IMAGE PIXEL MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Samples per Pixel	(0028,0002)	1	The value is set to 1.
Photometric Interpretation	(0028,0004)	1	The value is set to "MONOCHROME2".

Rows	(0028,0010)	1	This value is set to 1000. Note: For dose summary snapshot, this value will be 1024.
Columns	(0028,0011)	1	This value is set to 1000. Note: For dose summary snapshot, this value will be 980.
Bits Allocated	(0028,0100)	1	This value is set to 16. Note: For dose summary snapshot, this value will be 8.
Bits Stored	(0028,0101)	1	This value is set to 12. Note: For dose summary snapshot, this value will be 8.
High Bit	(0028,0102)	1	This value is set to 11. Note: For dose summary snapshot, this value will be 7.
Pixel Representation	(0028,0103)	1	This value is set to 0 for unsigned integer.
Pixel Data	(7FE0,0010)	1	Pixel data of the image.
Planar Configuration	(0028,0006)	1C	Not Used
Pixel Aspect Ratio	(0028,0034)	1C	Not Used
Smallest Image Pixel Value	(0028,0106)	3	Not Used
Largest Image Pixel Value	(0028,0107)	3	Not Used
Red Palette Color Lookup Table Descriptor	(0028,1101)	1C	Not Used
Green Palette Color Lookup Table Descriptor	(0028,1102)	1C	Not Used
Blue Palette Color Lookup Table Descriptor	(0028,1103)	1C	Not Used
Red Palette Color Lookup Table Data	(0028,1201)	1C	Not Used
Green Palette Color Lookup Table Data	(0028,1202)	1C	Not Used
Blue Palette Color Lookup Table Data	(0028,1203)	1C	Not Used
ICC Profile	(0028,2000)	3	Not Used
Pixel Data Provider URL	(0028,7FE0)	1C	Not Used
Pixel Padding Range Limit	(0028,0121)	1C	Not Used

4.4.5.3 Contrast/Bolus Module

TABLE 4-9
CONTRAST/BOLUS MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Contrast/Bolus Agent	(0018,0010)	2	Got from MWL, else, set as empty.
Contrast/Bolus Agent Sequence	(0018,0012)	3	Not Used
>Include 'Code Sequence Macro'			

Contrast/Bolus Route	(0018,1040)	3	Not Used
Contrast/Bolus Administration Route Sequence	(0018,0014)	3	Not Used
>Include 'Code Sequence Macro'			
>Additional Drug Sequence	(0018,002A)	3	Not Used
>>Include 'Code Sequence Macro'			
Contrast/Bolus Volume	(0018,1041)	3	Not Used
Contrast/Bolus Start Time	(0018,1042)	3	Not Used
Contrast/Bolus Stop Time	(0018,1043)	3	Not Used
Contrast/Bolus Total Dose	(0018,1044)	3	Not Used
Contrast Flow Rate(s)	(0018,1046)	3	Not Used
Contrast Flow Duration(s)	(0018,1047)	3	Not Used
Contrast/Bolus Ingredient	(0018,1048)	3	Not Used
Contrast/Bolus Ingredient Concentration	(0018,1049)	3	Not Used

4.4.5.4 X-Ray Image Module

TABLE 4-10
X-RAY IMAGE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Frame Increment Pointer	(0028,0009)	1C	Not Used
Lossy Image Compression	(0028,2110)	1C	Not Used
Image Type	(0008,0008)	1	See 4.4.5.4.1
Pixel Intensity Relationship	(0028,1040)	1	Value is DISP
Samples per Pixel	(0028,0002)	1	Value is 1
Photometric Interpretation	(0028,0004)	1	Value is MONOCHROME2
Bits Allocated	(0028,0100)	1	Value is 16. Note: For dose summary snapshot, this value will be 8.
Bits Stored	(0028,0101)	1	Value is 12. Note: For dose summary snapshot, this value will be 8.
High Bit	(0028,0102)	1	Value is 11. Note: For dose summary snapshot, this value will be 7.
Pixel Representation	(0028, 0103)	1	Value is 0000H
Scan Options	(0018,0022)	3	Not Used.
Anatomic Region Sequence	(0008,2218)	3	Not Used.
> Include 'Code Sequence Macro'			
>Anatomic Region Modifier Sequence	(0008,2220)	3	Not Used
>> Include 'Code Sequence Macro'			

Primary Anatomic Structure Sequence	(0008,2228)	3	Not Used
> Include 'Code Sequence Macro'			
>Primary Anatomic Structure Modifier Sequence	(0008,2230)	3	Not Used
>> Include 'Code Sequence Macro'			
R Wave Pointer	(0028,6040)	3	Not Used
Reference Image Sequence	(0008,1140)	1C	Not Used
>Referenced SOP Class UID	(0008,1150)	1	Not Used
>Referenced SOP Class UID	(0008,1155)	1	Not Used
>Referenced Frame Number	(0008,1160)	1C	Not Used
>Referenced Segment Number	(0062,000B)	1C	Not Used
>Purpose of Reference Code Sequence	(0040,A170)	3	Not Used
>> Include 'Code Sequence Macro'			
Derivation Description	(0008,2111)	3	Not Used
Acquisition Device Processing Description	(0018,1400)	3	Not Used
Frame Label Vector	(0018,2002)	3	Not Used
Frame Dimension Pointer	(0028,000A)	3	Not Used
Calibration Image	(0050,0004)	3	Not Used

4.4.5.4.1 Image Type

Define the values of Image Type (0008,0008) that may be sent and under what circumstances, or refer to the more general description in the General Image Module.

Value 1 shall have the following Enumerated Values:

- ORIGINAL identifies an Original Image
- DERIVED identifies a Derived Image.

Value 2 shall have the following Enumerated Value:

- PRIMARY identifies a Primary Image
- SECONDARY identifies a Secondary Image.

Specify which Enumerated Values of Value 3 are created/supported:

- SINGLE PLANE

4.4.5.5 X-Ray Acquisition Module

TABLE 4-11
X-RAY ACQUISITION MODULE

Attribute Name	Tag	Type	Attribute Description
KVP	(0018,0060)	2	KVP of the shot.
Radiation Setting	(0018,1155)	1	Fixed as "GR"
X-Ray Tube Current	(0018,1151)	2C	Used
X-Ray Tube Current in μ A	(0018,8151)	3	Used
Exposure Time	(0018,1150)	2C	mSec of the shot.
Exposure Time in μ S	(0018,8150)	3	Not Used

Exposure	(0018,1152)	2C	Not Used
Exposure in microAs	(0018,1153)	3	Not Used
Grid	(0018,1166)	3	Not Used
Average Pulse Width	(0018,1154)	3	Not Used
Radiation Mode	(0018,115A)	3	Fixed as “CONTINUOUS”
Type of Filters	(0018,1161)	3	Not Used
Intensifier Size	(0018,1162)	3	Not Used
Field of View Shape	(0018,1147)	3	Not Used
Field of View Dimension(s)	(0018,1149)	3	Not Used
Imager Pixel Spacing	(0018,1164)	3	Not Used
Pixel Spacing	(0028,0030)	1C	Not Used
Pixel Spacing Calibration Type	(0028,0A02)	3	Not Used
Pixel Spacing Calibration Description	(0028,0A04)	1C	Not Used
Focal Spot	(0018,1190)	3	Not Used
Image and Fluoroscopy Area Dose Product	(0018,115E)	3	DAP of the exam.

4.4.5.6 XA Positioner Module

TABLE 4-12
XA POSITIONER MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Distance Source to Patient	(0018,1111)	3	Not Used
Distance Source to Detector	(0018,1110)	3	447mm.
Estimated Radiographic Magnification Factor	(0018,1114)	3	Not Used
Positioner Motion	(0018,1500)	2C	Not Used
Positioner Primary Angle	(0018,1510)	2	Send with empty.
Positioner Secondary Angle	(0018,1511)	2	Send with empty.
Positioner Primary Angle Increment	(0018,1520)	2C	Not Used
Positioner Secondary Angle Increment	(0018,1521)	2C	Not Used
Detector Primary Angle	(0018,1530)	3	Not Used
Detector Secondary Angle	(0018,1531)	3	Not Used

4.4.5.7 Overlay Plane Module

The product supports up to 1 overlay in an image.

TABLE 4-13
OVERLAY PLANE MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Overlay Rows	(60xx,0010)	1	Value is 1000.
Overlay Columns	(60xx,0011)	1	Value is 1000.
Overlay Type	(60xx,0040)	1	Value is G.
Overlay Origin	(60xx,0050)	1	Value is 0\0.
Overlay Bits Allocated	(60xx,0100)	1	1
Overlay Bit Position	(60xx,0102)	1	0
Overlay Data	(60xx,3000)	1	Overlay pixel data
Overlay Description	(60xx,0022)	3	Value is "Annotation/Measurement Graphic Layer".
Overlay Subtype	(60xx,0045)	3	Not Used
Overlay Label	(60xx,1500)	3	Value is "Annotation/Measurement Graphic Layer".
ROI Area	(60xx,1301)	3	Not Used
ROI Mean	(60xx,1302)	3	Not Used
ROI Standard Deviation	(60xx,1303)	3	Not Used

4.4.5.8 VOI LUT module

TABLE 4-14
VOI LUT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
VOI LUT Sequence	(0028,3010)	1C	Not Used
>LUT Descriptor	(0028,3002)	1	Not Used
>LUT Explanation	(0028,3003)	3	Not Used
>LUT Data	(0028,3006)	1	Not Used
Window Center	(0028,1050)	1C	Only one value is present. Set to $2^{\wedge}bitsStored/2$ when export to DICOM images
Window Width	(0028,1051)	1C	Only one value is present. Set to $2^{\wedge}bitsStored-1$ when export to DICOM images
Window Center & Width Explanation	(0028,1055)	3	Not Used

4.4.5.9 SOP Common Module

TABLE 4-15
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
SOP Class UID	(0008,0016)	1	SOP Class UID for the Class that the dataset contains, just XA UID.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

SOP Instance UID	(0008,0018)	1	Created by equipment, using prefix: 1.2.840.113619.2.403. +MAC+imageIndicator(40)+TimeStamp_Exam MAC: Number string of device MAC address.
Specific Character Set	(0008,0005)	1C	Always set to ISO_IR 100(= Latin Alphabet No. 1)
Instance Creation Date	(0008,0012)	3	Not Used
Instance Creation Time	(0008,0013)	3	Not Used
Instance Creator UID	(0008,0014)	3	Not Used
Related General SOP Class UID	(0008,001A)	3	Not Used
Original Specialized SOP Class UID	(0008,001B)	3	Not Used
Coding Scheme Identification Sequence	(0008,0110)	3	Not Used
>Coding Scheme Designator	(0008,0102)	1	Not Used
>Coding Scheme Registry	(0008,0112)	1C	Not Used
>Coding Scheme UID	(0008,010C)	1C	Not Used
>Coding Scheme External ID	(0008,0114)	2C	Not Used
>Coding Scheme Name	(0008,0115)	3	Not Used
>Coding Scheme Version	(0008,0103)	3	Not Used
>Coding Scheme Responsible Organization	(0008,0116)	3	Not Used
Timezone Offset From UTC	(0008,0201)	3	Not Used
Contributing Equipment Sequence	(0018,A001)	3	Not Used
>Purpose of Reference Code Sequence	(0040,A170)	1	Not Used
>>Include 'Code Sequence Macro'			
>Manufacturer	(0008,0070)	1	Not Used
>Institution Name	(0008,0080)	3	Not Used
>Institution Address	(0008,0081)	3	Not Used
>Station Name	(0008,1010)	3	Not Used
>Institutional Department Name	(0008,1040)	3	Not Used
>Manufacturer's Model Name	(0008,1090)	3	Not Used
>Device Serial Number	(0018,1000)	3	Not Used
>Software Versions	(0018,1020)	3	Not Used
>Spatial Resolution	(0018,1050)	3	Not Used
>Date of Last Calibration	(0018,1200)	3	Not Used
>Time of Last Calibration	(0018,1201)	3	Not Used
>Contribution DateTime	(0018,A002)	3	Not Used
>Contribution Description	(0018,A003)	3	Not Used
Instance Number	(0020,0013)	3	Image number.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

SOP Instance Status	(0100,0410)	3	Not Used
SOP Authorization Date and Time	(0100,0420)	3	Not Used
SOP Authorization Comment	(0100,0424)	3	Not Used
Authorization Equipment Certification Number	(0100,0426)	3	Not Used
MAC Parameters Sequence	(4FFE,0001)	3	Not Used
>MAC ID Number	(0400,0005)	1	Not Used
>MAC Calculation Transfer Syntax UID	(0400,0010)	1	Not Used
>MAC Algorithm	(0400,0015)	1	Not Used
>Data Elements Signed	(0400,0020)	1	Not Used
Digital Signatures Sequence	(FFFA,FFFA)	3	Not Used
>MAC ID Number	(0400,0005)	1	Not Used
>Digital Signature UID	(0400,0100)	1	Not Used
>Digital Signature DateTime	(0400,0105)	1	Not Used
>Certificate Type	(0400,0110)	1	Not Used
>Certificate of Signer	(0400,0115)	1	Not Used
>Signature	(0400,0120)	1	Not Used
>Certified Timestamp Type	(0400,0305)	1C	Not Used
>Certified Timestamp	(0400,0310)	3	Not Used
>Digital Signature Purpose Code Sequence	(0400,0401)	3	Not Used
>>Include 'Code Sequence Macro'			
Encrypted Attributes Sequence	(0400,0500)	1C	Not Used
>Encrypted Content Transfer Syntax UID	(0400,0510)	1	Not Used
>Encrypted Content	(0400,0520)	1	Not Used
Original Attributes Sequence	(0400,0561)	3	Not Used
>Source of Previous Values	(0400,0564)	2	Not Used
>Attribute Modification DateTime	(0400,0562)	1	Not Used
>Modifying System	(0400,0563)	1	Not Used
>Reason for the Attribute Modification	(0400,0565)	1	Not Used
>Modified Attributes Sequence	(0400,0550)	1	Not Used
>>Any Attribute from the main data set that was modified or removed; may include Sequence Attributes and their Items.			
HL7 Structured Document Reference Sequence	(0040,A390)	1C	Not Used
>Referenced SOP Class UID	(0008,1150)	1	Not Used
>Referenced SOP Instance UID	(0008,1155)	1	Not Used
>HL7 Instance Identifier	(0040,E001)	1	Not Used
>Retrieve URI	(0040,E010)	3	Not Used

Longitudinal Temporal Information Modified	(0028,0303)	3	Used. If Include Remove Patient Information then fix to "MODIFIED".
--	-------------	---	--

4.5 STANDARD EXTENDED AND PRIVATE DATA ATTRIBUTES

Not applicable

4.5.1 Standard Attributes

Not applicable

4.6 STANDARD EXTENDED AND PRIVATE CONTEXT GROUPS

Not applicable

5. X-RAY RADIATION DOSE STRUCTURED REPORT INFORMATION OBJECT IMPLEMENTATION

5.1 INTRODUCTION

This section specifies the use of the DICOM X-Ray Radiation Dose SR IOD to represent results produced and/or received by this implementation. Corresponding attributes are conveyed using the module construct.

5.2 OEC ELITE MINIVIEW MAPPING OF DICOM ENTITIES

The OEC Elite MiniView maps DICOM Information Entities to local Information Entities in the product's database and user interface.

TABLE 5-1
MAPPING OF DICOM ENTITIES TO OEC ELITE MINIVIEW ENTITIES

DICOM IE	OEC Elite MiniView Entity
Patient	Patient
Study	Exam
Series	Series
Equipment	Equipment
Document	Document

5.3 IOD MODULE TABLE

The X-Ray Radiation Dose Structured Report Information Object Definitions comprise the modules of the following tables, plus Standard Extended and Private Attributes. Standard Extended and Private Attributes are described in Section 5.5

The contents of the SR Document Content are constrained by the supported template, as identified in Section 5.4.5.2.1.1. Standard, Standard Extended and Private Templates are further described in Section 5.7.

TABLE 5-2
STRUCTURE REPORT IOD MODULES

Entity Name	Module Name	Usage	Reference
Patient	Patient	Used	5.4.1.1
	Specimen Identification	Not Used	N/A
	Clinical Trial Subject	Not Used	N/A
Study	General Study	Used	5.4.2.1
	Patient Study	Used	5.4.2.2
	Clinical Trial Study	Not Used	N/A

Series	SR Document Series	Used	5.4.3.1
	Clinical Trial Series	Not Used	N/A
Frame Of Reference	Synchronization	Not Used	N/A
Equipment	General Equipment	Used	5.4.4.1
Document	SR Document General	Used	5.4.5.1
	SR Document Content	Used	5.4.5.2
	SOP Common	Used	5.4.5.3

5.4 INFORMATION MODULE DEFINITIONS

Please refer to DICOM Part 3 (Information Object Definitions) for a description of each of the entities, modules, and attributes contained within the SR Information Objects.

The following modules are included to convey Enumerated Values, Defined Terms, and Optional Attributes supported and/or expected. Type 1 & Type 2 Attributes are also included for completeness and to define what values they may take and where these values are obtained from when generating the instance as well as what are the expected values when loading such instance. It should be noted that they are the same ones as defined in the DICOM Standard Part 3 (Information Object Definitions). Also note that Attributes not present in tables are not supported.

5.4.1 Patient Entity Modules

5.4.1.1 Patient Module

TABLE 5-3
PATIENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Patient's Name	(0010,0010)	2	May be entered from user interface or got from Worklist. Supports 5 different components delimited by “^”, 64 bytes maximum per component group.
Patient ID	(0010,0020)	2	May be entered from user interface or got from Worklist. Truncated to 64 bytes, end truncated.
Issuer of Patient ID	(0010,0021)	3	Got from Worklist. Truncated to 64 bytes, end truncated.
Patient's Birth Date	(0010,0030)	2	May be entered from user interface or got from Worklist Truncated to 8 bytes, end truncated
Patient's Sex	(0010,0040)	2	May be entered from user interface or got from Worklist. Truncated to 2 bytes, end truncated
Referenced Patient Sequence	(0008,1120)	3	Not Used

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

>Include 'SOP Instance Reference Macro'			
Patient's Birth Time	(0010,0032)	3	Not Used
Other Patient IDs	(0010,1000)	3	Not Used
Other Patient IDs Sequence	(0010,1002)	3	Not Used
>Patient ID	(0010,0020)	1	Not Used
>Issuer of Patient ID	(0010,0021)	1	Not Used
>Type of Patient ID	(0010,0022)	1	Not Used
Other Patient Names	(0010,1001)	3	Not Used
Ethnic Group	(0010,2160)	3	Not Used
Patient Comments	(0010,4000)	3	May be entered from user interface or got from Worklist From user interface truncated to 512 bytes. From worklist truncated to 10240 bytes.
Patient Species Description	(0010,2201)	1C	Not Used
Patient Species Code Sequence	(0010,2202)	1C	Not Used
>Include 'Code Sequence Macro'			
Patient Breed Description	(0010,2292)	2C	Not Used
Patient Breed Code Sequence	(0010,2293)	2C	Not Used
>Include 'Code Sequence Macro'			
Breed Registration Sequence	(0010,2294)	2C	Not Used
>Breed Registration Number	(0010,2295)	1	Not Used
>Breed Registry Code Sequence	(0010,2296)	1	Not Used
>>Include 'Code Sequence Macro'			
Responsible Person	(0010,2297)	2C	Not Used
Responsible Person Role	(0010,2298)	1C	Not Used
Responsible Organization	(0010,2299)	2C	Not Used
Patient Identity Removed	(0012,0062)	3	Used. If Patient Information is removed then set to "YES", otherwise set to "NO"
De-identification Method	(0012,0063)	1C	Used. If Patient Information is removed. Set to "Limited Data Set" in this case
De-identification Method Code Sequence	(0012,0064)	1C	Not Used
>Include 'Code Sequence Macro'			

GE Healthcare

1694829 REV 3

5.4.2 Study Entity Modules

5.4.2.1 General Study Module

TABLE 5-4
GENERAL STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Study Instance UID	(0020,000D)	1	The product will adopt the Study Instance UID which is returned in the MWL response. If there is no Study Instance UID returned from MWL server, then new Study Instance UID will be created.
Study Date	(0008,0020)	2	This value is set to the exam created date.
Study Time	(0008,0030)	2	This value is set to the exam created time.
Referring Physician's Name	(0008,0090)	2	Got from Worklist.
Referring Physician Identification Sequence	(0008,0096)	3	Not Used
>Include 'Person Identification Macro'			
Study ID	(0020,0010)	2	Generated by equipment.
Accession Number	(0008,0050)	2	May be entered from the user interface or got from Worklist.
Study Description	(0008,1030)	3	May be entered from the user interface or got from Worklist. The default value will be set as Requested Procedure Description when the tag got from MWL is not empty. Else this value will be set as Procedure Description on user interface.
Physician(s) of Record	(0008,1048)	3	Not Used
Physician(s) of Record Identification Sequence	(0008,1049)	3	Not Used
>Include 'Person Identification Macro'			
Name of Physician(s) Reading Study	(0008,1060)	3	Not Used
Physician(s) Reading Study Identification Sequence	(0008,1062)	3	Not Used
>Include 'Person Identification Macro'			
Referenced Study Sequence	(0008,1110)	3	Got from Worklist.
>Include 'SOP Instance Reference Macro'			
Procedure Code Sequence	(0008,1032)	3	Not Used
>Include 'Code Sequence Macro'			

5.4.2.2 Patient Study Module

TABLE 5-5
PATIENT STUDY MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
----------------	-----	------	-----------------------

Admitting Diagnoses Description	(0008,1080)	3	Not Used
Admitting Diagnoses Code Sequence	(0008,1084)	3	Not Used
>Include 'Code Sequence Macro'			
Patient's Age	(0010,1010)	3	Not Used
Patient's Size	(0010,1020)	3	Used
Patient's Weight	(0010,1030)	3	Used
Occupation	(0010,2180)	3	Not Used
Additional Patient's History	(0010,21B0)	3	Not Used
Admission ID	(0038,0010)	3	Not Used
Issuer of Admission ID	(0038,0011)	3	Not Used
Service Episode ID	(0038,0060)	3	Not Used
Issuer of Service Episode ID	(0038,0061)	3	Not Used
Service Episode Description	(0038,0062)	3	Not Used
Patient's Sex Neutered	(0010,2203)	2C	Not Used

5.4.3 Series Entity Modules

5.4.3.1 SR Document Series Module

TABLE 5-6
SR DOCUMENT SERIES MODULE ATTRIBUTES

Attribute Name	Tag	Type	Use
Modality	(0008,0060)	1	Value = SR
Series Instance UID	(0020,000E)	1	Created by equipment, using prefix: 1.2.840.113619.2.403. +MAC+seriesIndicator(21)+TimeStamp_Exam MAC: Number string of device MAC address.
Series Number	(0020,0011)	1	A number that identifies this Series. This number will be set to 1 for image series and set to 2 for RDSR series
Series Date	(0008,0021)	3	First shot date.
Series Time	(0008,0031)	3	First shot time.
Series Description	(0008,103E)	3	The value equal protocol Name.
Referenced Performed Procedure Step Sequence	(0008,1111)	2	Always send. Referenced SOP Class UID = MPPS SOP Class UID. Referenced SOP Instance UID = MPPS SOP Instance UID.
> 'Referenced SOP Class / Instance UIDs'			

GE Healthcare

1694829 REV 3

5.4.4 Equipment Entity Modules

5.4.4.1 General Equipment Module

TABLE 5-7
GENERAL EQUIPMENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
Manufacturer	(0008,0070)	2	This value is set to "GE Hualun Medical Systems, Co. Ltd".
Institution Name	(0008,0080)	3	Configurable by user on setup screen (The field name is "Hospital Name").
Institution Address	(0008,0081)	3	Not Used
Station Name	(0008,1010)	3	Configurable by user on DICOM setup screen.
Institutional Department Name	(0008,1040)	3	Not Used
Manufacturer's Model Name	(0008,1090)	3	This value is set to type and model of the system: "OEC Elite MiniView".
Device Serial Number	(0018,1000)	3	Configurable during system installation.
Software Versions	(0018,1020)	3	This value is set to workstation software version.
Gantry ID	(0018,1008)	3	Not Used
Spatial Resolution	(0018,1050)	3	Not Used
Date of Last Calibration	(0018,1200)	3	Not Used
Time of Last Calibration	(0018,1201)	3	Not Used
Pixel Padding Value	(0028,0120)	1C	Not Used

5.4.5 Document Entity Modules

5.4.5.1 SR Document General Module

TABLE 5-8
SR DOCUMENT GENERAL MODULE ATTRIBUTES

Attribute Name	Tag	Type	Use
Instance Number	(0020,0013)	1	Value is 1.
Completion Flag	(0040,A491)	1	COMPLETE
Completion Flag Description	(0040,A492)	3	Not Used
Verification Flag	(0040,A493)	1	UNVERIFIED
Content Date	(0008,0023)	1	First shot date.
Content Time	(0008,0033)	1	First shot time.
Verifying Observer Sequence	(0040,A073)	1C	Not Used.
>Verifying Observer Name	(0040,A075)	1	Not Used
>Verifying Observer Identification Code Sequence	(0040,A088)	2	Not Used
>>Include 'Code Sequence Macro'			
>Verifying Organization	(0040,A027)	1	Not Used
>Verification DateTime	(0040,A030)	1	Not Used

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare
1694829 REV 3

Author Observer Sequence	(0040,A078)	3	Used
>Include 'Identified Person or Device Macro'			
Participant Sequence	(0040,A07A)	3	Not Used
>Participation Type	(0040,A080)	1	Not Used
>Participation DateTime	(0040,A082)	2	Not Used
>Include 'Identified Person or Device Macro'			
Custodial Organization Sequence	(0040,A07C)	3	Not Used
>Institution Name	(0008,0080)	2	Not Used
>Institution Code Sequence	(0008,0082)	2	Not Used
>>Include 'Code Sequence Macro'			
Predecessor Documents Sequence	(0040,A360)	1C	Not Used
>Include 'Hierarchical SOP Instance Reference Macro'			
Identical Documents Sequence	(0040,A525)	1C	Not Used
>Include 'Hierarchical SOP Instance Reference Macro'			
Referenced Request Sequence	(0040,A370)	1C	Used
>Study Instance UID	(0020,000D)	1	The product will adopt the Study Instance UID which is returned in the MWL response. If there is no Study Instance UID returned from MWL server, then new Study Instance UID will be created by system during exam creation.
>Referenced Study Sequence	(0008,1110)	2	Set as empty
>>Include 'SOP Instance Reference Macro'			
>Accession Number	(0008,0050)	2	The product will adopt the Accession Number which is returned in the MWL response. If there is no Accession Number returned from MWL server, then the value will keep empty. For local created exam, user could input value from screen during exam creation.
>Placer Order Number/Imaging Service Request	(0040,2016)	2	Value is empty.
>Filler Order Number/Imaging Service Request	(0040,2017)	2	Value is empty.
>Requested Procedure ID	(0040,1001)	2	This value could got from MWL response. If not contained in MWL response, then keep empty as default.
>Requested Procedure Description	(0032,1060)	2	This value could got from MWL response. If not contained in MWL response, then keep empty as default.
>Requested Procedure Code Sequence	(0032,1064)	2	Value is empty.
>>Include 'Code Sequence Macro'			
>Reason for the Requested Procedure	(0040,1002)	3	Not Used
>Reason for Requested Procedure Code Sequence	(0040,100A)	3	Not Used
>>Include 'Code Sequence Macro'			

Performed Procedure Code Sequence	(0040,A372)	2	Empty.
>Include Code Sequence Macro			
Current Requested Procedure Evidence Sequence	(0040,A375)	1C	With the value(s) from the system of all saved images for the exam. This is the list of all images whether they have been stored to PACS or not.
>Include 'Hierarchical SOP Instance Reference Macro'			
Pertinent Other Evidence Sequence	(0040,A385)	1C	Not Used
> Include 'Hierarchical SOP Instance Reference Macro'			
Referenced Instance Sequence	(0008,114A)	1C	Not Used
>Include 'SOP Instance Reference Macro'			
>Purpose of Reference Code Sequence	(0040,A170)	1	Not Used
>>Include 'Code Sequence Macro'			

5.4.5.2 SR Document Content Module

TABLE 5-9
SR DOCUMENT CONTENT MODULE ATTRIBUTES

Attribute Name	Tag	Type	Use
Observation DateTime	(0040,A032)	1C	Not Used
Content Template Sequence	(0040,A504)	1C	Not Used
>Mapping Resource	(0008,0105)	1	Not Used
>Template Identifier	(0040,DB00)	1	Not Used
Value Type	(0040,A040)	1	CONTAINER
Continuity of Content	(0040,A050)	1C	SEPARATE
Concept Name Code Sequence	(0040,A043)	1C	Used
>Include 'Code Sequence Macro'			
Insert Concept Value attribute(s)			(113701,DCM, X-Ray Radiation Dose Report)
Content Sequence	(0040,A730)	1C	Used
> Relationship Type	(0040,A010)	1	HAS CONCEPT MOD
> Referenced Content Item Identifier	(0040,DB73)	1C	Not Used
> Insert SR DocumentContent Module			Recursive inclusion to create document content tree. See section 5.4.5.2.1 for the list of supported templates

5.4.5.2.1 SR Document Content Descriptions

5.4.5.2.1.1 Content Template

The product supports the following root Templates for SR SOP Instances created, processed, or displayed by the product.

TABLE 5-10
SR ROOT TEMPLATES

SOP Class	Template ID	Template Name	Use
X-Ray Radiation Dose SR	10001	X-Ray Radiation Dose	Create/Display

Refer to section 5.7 for a detailed description of the supported templates.

5.4.5.3 SOP Common Module

TABLE 5-41
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Type	Attribute Description
SOP Class UID	(0008,0016)	1	SOP Class UID for the Class that the dataset contains, just RDSR UID.
SOP Instance UID	(0008,0018)	1	Created by equipment, using prefix: 1.2.840.113619.2.403. +MAC+imageIndicator(50)+TimeStamp_Exam MAC: Number string of device MAC address.
Specific Character Set	(0008,0005)	1C	Always set to ISO_IR 100(= Latin Alphabet No. 1)
Instance Creation Date	(0008,0012)	3	Used
Instance Creation Time	(0008,0013)	3	Used
Instance Creator UID	(0008,0014)	3	Used
Related General SOP Class UID	(0008,001A)	3	Not Used
Original Specialized SOP Class UID	(0008,001B)	3	Not Used
Coding Scheme Identification Sequence	(0008,0110)	3	Not Used
>Coding Scheme Designator	(0008,0102)	1	Not Used
>Coding Scheme Registry	(0008,0112)	1C	Not Used
>Coding Scheme UID	(0008,010C)	1C	Not Used
>Coding Scheme External ID	(0008,0114)	2C	Not Used
>Coding Scheme Name	(0008,0115)	3	Not Used
>Coding Scheme Version	(0008,0103)	3	Not Used
>Coding Scheme Responsible Organization	(0008,0116)	3	Not Used
Timezone Offset From UTC	(0008,0201)	3	Not Used
Contributing Equipment Sequence	(0018,A001)	3	Not Used
>Purpose of Reference Code Sequence	(0040,A170)	1	Not Used
>>Include 'Code Sequence Macro'			
>Manufacturer	(0008,0070)	1	Not Used
>Institution Name	(0008,0080)	3	Not Used
>Institution Address	(0008,0081)	3	Not Used

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

>Station Name	(0008,1010)	3	Not Used
>Institutional Department Name	(0008,1040)	3	Not Used
>Manufacturer's Model Name	(0008,1090)	3	Not Used
>Device Serial Number	(0018,1000)	3	Not Used
>Software Versions	(0018,1020)	3	Not Used
>Spatial Resolution	(0018,1050)	3	Not Used
>Date of Last Calibration	(0018,1200)	3	Not Used
>Time of Last Calibration	(0018,1201)	3	Not Used
>Contribution DateTime	(0018,A002)	3	Not Used
>Contribution Description	(0018,A003)	3	Not Used
Instance Number	(0020,0013)	3	Image number.
SOP Instance Status	(0100,0410)	3	Not Used
SOP Authorization Date and Time	(0100,0420)	3	Not Used
SOP Authorization Comment	(0100,0424)	3	Not Used
Authorization Equipment Certification Number	(0100,0426)	3	Not Used
MAC Parameters Sequence	(4FFE,0001)	3	Not Used
>MAC ID Number	(0400,0005)	1	Not Used
>MAC Calculation Transfer Syntax UID	(0400,0010)	1	Not Used
>MAC Algorithm	(0400,0015)	1	Not Used
>Data Elements Signed	(0400,0020)	1	Not Used
Digital Signatures Sequence	(FFFA,FFFA)	3	Not Used
>MAC ID Number	(0400,0005)	1	Not Used
>Digital Signature UID	(0400,0100)	1	Not Used
>Digital Signature DateTime	(0400,0105)	1	Not Used
>Certificate Type	(0400,0110)	1	Not Used
>Certificate of Signer	(0400,0115)	1	Not Used
>Signature	(0400,0120)	1	Not Used
>Certified Timestamp Type	(0400,0305)	1C	Not Used
>Certified Timestamp	(0400,0310)	3	Not Used
>Digital Signature Purpose Code Sequence	(0400,0401)	3	Not Used
>>Include 'Code Sequence Macro'			
Encrypted Attributes Sequence	(0400,0500)	1C	Not Used
>Encrypted Content Transfer Syntax UID	(0400,0510)	1	Not Used
>Encrypted Content	(0400,0520)	1	Not Used
Original Attributes Sequence	(0400,0561)	3	Not Used
>Source of Previous Values	(0400,0564)	2	Not Used
>Attribute Modification DateTime	(0400,0562)	1	Not Used

>Modifying System	(0400,0563)	1	Not Used
>Reason for the Attribute Modification	(0400,0565)	1	Not Used
>Modified Attributes Sequence	(0400,0550)	1	Not Used
>>Any Attribute from the main data set that was modified or removed; may include Sequence Attributes and their Items.			
HL7 Structured Document Reference Sequence	(0040,A390)	1C	Not Used
>Referenced SOP Class UID	(0008,1150)	1	Not Used
>Referenced SOP Instance UID	(0008,1155)	1	Not Used
>HL7 Instance Identifier	(0040,E001)	1	Not Used
>Retrieve URI	(0040,E010)	3	Not Used
Longitudinal Temporal Information Modified	(0028,0303)	3	Used. If Include Remove Patient Information then fix to "MODIFIED".

5.5 STANDARD EXTENDED AND PRIVATE DATA ATTRIBUTES

Not applicable

5.6 STANDARD EXTENDED AND PRIVATE CONTEXT GROUPS

The Product supports coded terminology using Standard Extended, Private, and Configurable Context Groups defined in the following sections.

5.6.1 Standard Extended Context Groups

The Product supports the following extensions to standard Context Groups for SR SOP Instances created by this product. Extensions are indicated by **bold text**.

5.6.2 Configurable Context Groups

The Product supports the following Configurable Context Groups for SR SOP Instances created by this product.

Context Group	Default Value Set	Use
N/A	N/A	N/A

5.7 STANDARD, STANDARD EXTENDED AND PRIVATE TEMPLATES

The Product supports the Standard Extended and Private Templates defined in the following sections.

5.7.1 Standard Templates

The Product supports the following standard templates for SOP Instances created by this product.

GE Healthcare

1694829 REV 3

5.7.1.1 Template ID 10001 X-Ray Radiation Dose

TID 10001

PROJECTION X-RAY RADIATION DOSE

Type: Extensible Order: Significant

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV (113701, DCM, "X-Ray Radiation Dose Report")	1	M		Root Node
2	>	HAS CONCEPT MOD	CODE	EV (121058, DCM, "Procedure reported")	1	M		DT (113704, DCM, "Projection X-Ray")
3	>>	HAS CONCEPT MOD	CODE	EV (G-C0E8, SRT, "Has Intent")	1	M		(R-408C3,SRT,Diagnostic Intent)
4	>		INCLUDE	DTID (1002) Observer Context	1-n	M		
5	>	HAS OBS CONTEXT	CODE	EV (113705, DCM, "Scope of Accumulation")	1	M		(113016, DCM, "Performed Procedure Step").
6	>>	HAS PROPERTIES	UIDREF	DCID (10001) UID Types	1	M		(121126, DCM, "Performed Procedure Step SOP Instance UID")
7	>	CONTAINS	INCLUDE	DTID (10002) Accumulated X-Ray Dose	1	MC	IFF Single Plane system	\$Plane = EV (113622, DCM, "Single Plane")
8	>	CONTAINS	INCLUDE	DTID (10002) Accumulated X-Ray Dose	1	MC	IFF Biplane system	Not Used
9	>	CONTAINS	INCLUDE	DTID (10002) Accumulated X-Ray Dose	1	MC	IFF Biplane system	Not Used
10	>	CONTAINS	INCLUDE	DTID (10003) Irradiation Event X-Ray Data	1-n	M		
11	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")	1	U		Patient Comment
12	>	CONTAINS	IMAGE	EV (121342, DCM, "Dose Image")	1-n	U		Not Used
13	>	CONTAINS	INCLUDE	DTID (1020) Person Participant	1	U		Not Used
14	>	CONTAINS	CODE	EV (113854, DCM, "Source of Dose Information")	1-n	M		(113856, DCM, "Automated Data Collection")

5.7.1.2 Template ID 10002 Accumulated X-Ray Dose

TID 10002
ACCUMULATED X-RAY DOSE
Type: Extensible Order: Significant

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV (113702, DCM, "Accumulated X-Ray Dose Data")	1	M		
2	>	HAS CONCEPT MOD	CODE	EV (113764, DCM, "Acquisition Plane")	1	M		(113622,DCM, "Single Plane")
3	>	CONTAINERS	CONTAINER	EV (122505, DCM, "Calibration")	1-n	MC	IFF Calibration Data is available	
4	>>	HAS CONCEPT MOD	CODE	EV (113794, DCM, "Dose Measurement Device")	1	M		(A-2C090, SRT, "Dosimeter")
5	>>	CONTAINERS	DATETIME	EV (113723, DCM, "Calibration Date")	1	M		The date of DAP Calibration performed.
6	>>	CONTAINERS	NUM	EV (122322, DCM, "Calibration Factor")	1	M		Units = EV (1, UCUM, "no units") Value is 1.
7	>>	CONTAINERS	NUM	EV (113763, DCM, "Calibration Uncertainty")	1	M		Units = EV (% , UCUM, "Percent") Value is 25%.
8	>>	CONTAINERS	TEXT	EV (113724, DCM, "Calibration Responsible Party")	1	M		Regional Sales Administrator (RSA)
9	>	CONTAINERS	INCLUDE	DTID (10004) Accumulated Projection X-Ray Dose	1	MC	XOR row 10, IFF TID (10001) Row 2 = (113704, DCM, "Projection X-Ray")	
10	>	CONTAINERS	INCLUDE	DTID (10005) Accumulated Mammography X-Ray Dose	1	MC	XOR row 9, IFF TID (10001) Row 2 = (P5-40010, SRT, "Mammography")	Not Used
11	>	CONTAINERS	INCLUDE	DTID (1021) Device	1	MC	Required if the irradiating device is	\$DeviceProcedureRole = EV (113859, DCM,

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare
1694829 REV 3

			Participant			not the recording device and the dose was accumulated on a single device.	"Irradiating Device")
--	--	--	-------------	--	--	---	-----------------------

5.7.1.3 Template ID 10003 Irradiation Event X-Ray Data

TID 10003

IRRADIATION EVENT X-RAY DATA

Type: Extensible Order: Significant

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV (113706, DCM, "Irradiation Event X-Ray Data")	1	M		
2	>	HAS CONCEPT MOD	CODE	EV (113764, DCM, "Acquisition Plane")	1	M		(113622, DCM, "Single Plane")
3	>	CONTAINS	DATETIME	DT (111526, DCM, "DateTime Started")	1	M		Date and time of first shot
4	>	CONTAINS	CODE	EV (113721, DCM, "Irradiation Event Type")	1	M		(P5-06000, SRT, "Fluoroscopy").
5	>	CONTAINS	TEXT	EV (125203, DCM, "Acquisition Protocol")	1	U		The text value of the IOD tag (0018,1030) Protocol Name from the system.
6	>	CONTAINS	CODE	EV (T-D0005, SRT, "Anatomical structure")	1	U		Not Used
7	>>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT, "Laterality")	1	UC	If anatomy is bi-lateral	Come from XA IOD (0020,0060) Laterality.
8	>	CONTAINS	TEXT	EV (113780, DCM, "Reference Point Definition")	1	MC	IF Row 13 or Row 14 is present and Row 9 is not present	The text value is "15cm in Front of Image Input Surface"
9	>	CONTAINS	CODE	EV (113780, DCM, "Reference Point Definition")	1	MC	IF Row 13 or Row 14 is present and Row 8 is not present	Not Used
10	>	CONTAINS	UIDREF	EV (113769, DCM, "Irradiation Event UID")	1	M		The UID value of the irradiation event from the system.
11	>	CONTAINS	NUM	EV (122130, DCM, "Dose Area Product")	1	MC	IFF TID (10001) Row 2 = (113704, DCM, "Projection X-Ray")	Units = EV (Gy.m2, UCUM, "Gy.m2")
12	>	CONTAINS	NUM	EV (111631,	1	MC	IFF TID (10001) Row	Not Used

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

		NS		DCM, "Average Glandular Dose")		2 = (P5-40010, SRT, "Mammography")	
13	>	CONTAIN NS	NUM	EV (113738, DCM, "Dose (RP)")	1	MC	Units = EV (Gy, UCUM, "Gy") Dose applied at the Reference Point (RP) IFF TID (10001) Row 2 = (113704, DCM, "Projection X-Ray") AND any of the values of TID (10001) Row 14 are not (113858, DCM, "MPPS Content")
14	>	CONTAIN NS	NUM	EV (111636, DCM, "Entrance Exposure at RP")	1	MC	IFF TID (10001) Row 2 = (P5-40010, SRT, "Mammography") Not Used
15	>	CONTAIN NS	NUM	EV (112011, DCM, "Positioner Primary Angle")	1	UC	XOR Row 19 Not Used
16	>	CONTAIN NS	NUM	EV (112012, DCM, "Positioner Secondary Angle")	1	UC	XOR Row 19 Not Used
17	>	CONTAIN NS	NUM	EV (113739, DCM, "Positioner Primary End Angle")	1	UC	IFF Row 4 value = (113613, DCM, "Rotational Acquisition") Not Used
18	>	CONTAIN NS	NUM	EV (113740, DCM, "Positioner Secondary End Angle")	1	UC	IFF Row 4 value = (113613, DCM, "Rotational Acquisition") Not Used
19	>	CONTAIN NS	NUM	EV (113770, DCM, "Column Angulation")	1	UC	XOR Rows 15,16 Not Used
20	>	CONTAIN NS	NUM	EV (113790, DCM, "Collimated Field Area")	1	U	Not Used
21	>	CONTAIN NS	CONTAINER	EV (113771, DCM, "X-Ray Filters")	1-n	U	Not Used
22	>>	CONTAIN NS	CODE	EV (113772, DCM, "X-Ray Filter Type")	1	U	Not Used
23	>>	CONTAIN NS	CODE	EV (113757, DCM, "X-Ray Filter Material")	1	U	Not Used
24	>>	CONTAIN NS	NUM	EV (113758, DCM, "X-Ray Filter Thickness Minimum")	1	U	Not Used
25	>>	CONTAIN NS	NUM	EV (113773, DCM, "X-Ray Filter Thickness Maximum")	1	U	Not Used
26	>	CONTAIN	CODE	EV (113732,	1	UC	IFF Row 4 value = The value of code (113630,

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

		NS		DCM, "Fluoro Mode")			(P5-06000, SRT, "Fluoroscopy")	DCM, "Continuous") for continuous mode irradiation events.
27	>	CONTAINNS	NUM	EV (113791, DCM, "Pulse Rate")	1	MC	IFF Row 26 value = (113631, DCM, "Pulsed")	Not Used
28	>	CONTAINNS	NUM	EV (113768, DCM, "Number of Pulses")	1	MC	IFF Row 26 value = (113631, DCM, "Pulsed")	Not Used
29	>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	1	MC	IFF count of pulses in Row 28 is estimated	Not Used
30	>	CONTAINNS	NUM	EV (113733, DCM, "KVP")	1-n	U		Units = EV (kV, UCUM, "kV") For Continuous mode irradiation events.
31	>	CONTAINNS	NUM	EV (113734, DCM, "X-Ray Tube Current")	1-n	U		Units = EV (mA, UCUM, "mA")
32	>	CONTAINNS	NUM	EV (113735, DCM, "Exposure Time")	1	U		Units = EV (ms, UCUM, "ms")
33	>	CONTAINNS	NUM	EV (113793, DCM, "Pulse Width")	1-n	U		Not Used
34	>	CONTAINNS	NUM	EV (113736, DCM, "Exposure")	1-n	U		Not Used
35	>	CONTAINNS	NUM	EV (113766, DCM, "Focal Spot Size")	1	U		Not Used
36	>	CONTAINNS	NUM	EV (113742, DCM, "Irradiation Duration")	1	U		Not Used
37	>	CONTAINNS	NUM	EV (113767, DCM, "Average X-Ray Tube Current")	1	U		Units = EV (mA, UCUM, "mA") The same with above "X-Ray Tube Current"
38	>	CONTAINNS	CODE	EV (113745, DCM, "Patient Table Relationship")	1	U		Not Used
39	>	CONTAINNS	CODE	EV (113743, DCM, "Patient Orientation")	1	U		Not Used
40	>>	HAS CONCEPT MOD	CODE	EV (113744, DCM, "Patient Orientation Modifier")	1	M		Not Used
41	>	CONTAINNS	NUM	DCID (10008) Dose Related	1-n	U		Not Used

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

		NS		Distance Measurements				
42	>	CONTAIN	NUM	EV (113754, DCM, "Table Head Tilt Angle")	1	U		Not Used
43	>	CONTAIN	NUM	EV (113755, DCM, "Table Horizontal Rotation Angle")	1	U		Not Used
44	>	CONTAIN	NUM	EV (113756, DCM, "Table Cradle Tilt Angle")	1	U		Not Used
45	>	CONTAIN	CODE	EV (123014, DCM, ("Target Region"))	1	M		1. The code from the system using DICOM Part 16 Context ID 4031 values and supporting the code (T-D0001, SRT, "Topography unknown") for an 'Unknown' value which is SNOMED term. 2. User could set this value in EM->Additional Screen Default is (T-D0001, SRT, "Topography unknown")
46	>	CONTAIN	CODE	EV (111632, DCM, "Anode Target Material")	1	U		Not Used
47	>	CONTAIN	NUM	EV (111633, DCM, "Compression Thickness")	1	U		Not Used
48	>	CONTAIN	NUM	EV (111634, DCM, "Half Value Layer")	1	U		Not Used
49	>	CONTAIN	CODE	EV (111635, DCM, "X-Ray Grid")	1-n	U		Not Used
50	>	CONTAIN	INCLUDE	DTID (4007) Mammography CAD Breast Composition	1	U		Not Used
51	>	CONTAIN	TEXT	EV (121106, DCM, "Comment")	1	U		Patient Comment
52	>	CONTAIN	INCLUDE	DTID (1020) Person Participant	1-n	U		Not Used
53	>	CONTAIN	INCLUDE	DTID (1021) Device Participant	1	MC	Required if the irradiating device is not the recording device.	Not Used
54	>	CONTAIN	IMAGE	EV (113795,	1-n	MC	IFF Image Object is	All image UUIDs.

GE Healthcare
1694829 REV 3

		NS		DCM, "Acquired Image")			created for this irradiation event	
55	>	CONTAI NS	NUM	EV (113845, DCM, "Exposure Index")	1	U		Not Used
56	>	CONTAI NS	NUM	EV (113846, DCM, "Target Exposure Index")	1	U		Not Used
57	>	CONTAI NS	NUM	EV (113847, DCM, "Deviation Index")	1	U		Not Used

5.7.1.4 Template ID 10004 Accumulated Projection X-Ray Dose

TID 10004
ACCUMULATED PROJECTION X-RAY DOSE
Type: Extensible Order: Significant

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			NUM	EV (113722, DCM, "Dose Area Product Total")	1	M		Units = EV (Gy.m2, UCUM, "Gy.m2") The numeric value of Total Dose Area Product. (Radioscopic)
2			NUM	EV (113725, DCM, "Dose (RP) Total")	1	MC	IF any of the values of TID (10001) Row 14 are not (113858, DCM, "MPPS Content"). May be present otherwise.	Units = EV (Gy, UCUM, "Gy") The numeric value of Cumulative Air Kerma.(Radioscopic)
3			NUM	EV (113726, DCM, "Fluoro Dose Area Product Total")	1	MC	IFF TID(10003) Row 4 value = (P5-06000, SRT, "Fluoroscopy") for at least one irradiation event	Units = EV (Gy.m2, UCUM, "Gy.m2") The numeric value of Total Radioscopic Dose Area Product.
4			NUM	EV (113728, DCM, "Fluoro Dose (RP) Total")	1	MC	IFF TID(10003) Row 4 value = (P5-06000, SRT, "Fluoroscopy") for at least one irradiation event AND any of the values of TID (10001) Row 14 are not (113858, DCM, "MPPS Content").	Units = EV (Gy, UCUM, "Gy") The numeric value of Cumulative Radioscopic Air Kerma.
5			NUM	EV (113730, DCM, "Total Fluoro Time")	1	MC	IFF TID(10003) Row 4 value = (P5-06000, SRT, "Fluoroscopy") for at least one irradiation event.	Units = EV (s, UCUM, "s") The numeric value of Total Radioscopic time to the second.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare
1694829 REV 3

6			NUM	EV (113727, DCM, "Acquisition Dose Area Product Total")	1	M		Units = EV (Gy.m2, UCUM, "Gy.m2") The numeric value of Total Radiographic Dose Area Product.
7			NUM	EV (113729, DCM, "Acquisition Dose (RP) Total")	1	MC	IF any of the values of TID (10001) Row 14 are not (113858, DCM, "MPPS Content"). May be present otherwise.	Units = EV (Gy, UCUM, "Gy") The numeric value of Cumulative Radiographic Air kerma.
8			NUM	EV (113855, DCM, "Total Acquisition Time")	1	M		Units = EV (s, UCUM, "s") The numeric value of Total Radiographic pedal time in milliseconds.
9			NUM	EV (113731, DCM, "Total Number of Radiographic Frames")	1	U		Not Used
10			CODE	EV (113780, DCM, "Reference Point Definition")	1	MC	IF Row 2, Row 4 or Row 7 is present and Row 11 is not present.	Not Used
11			TEXT	EV (113780, DCM, "Reference Point Definition")	1	MC	IF Row 2, Row 4 or Row 7 is present and Row 10 is not present.	The text value is "15cm in Front of Image Input Surface"

5.7.1.5 Template ID 1002 Observer Context

TID 1002
OBSERVER CONTEXT

Type: Non-Extensible Order: Significant

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1		HAS OBS CONTEXT	CODE	EV (121005,DCM, "Observer Type")	1	MC	IF Observer type is device	(121007, DCM, "Device")
2		HAS OBS CONTEXT	INCLUDE	DTID (1003) Person observer identifying attributes	1	MC	IFF Row 1 value = (121006,DCM, "Person") or Row 1 is absent	Not Used
3		HAS OBS CONTEXT	INCLUDE	DTID (1004) Device observer identifying attributes	1	MC	IFF Row 1 value = (121007,DCM, "Device")	

GE Healthcare

1694829 REV 3

5.7.1.6 Template ID 1004 Device Observer Identifying Attributes

TID 1004

DEVICE OBSERVER IDENTIFYING ATTRIBUTES

Type: Extensible Order: Significant

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			UIDREF	EV (121012,DCM, "Device Observer UID")	1	M		System Generated
2			TEXT	EV (121013,DCM, "Device Observer Name")	1	U		Defaults to value of Station Name (0008,1010) in General Equipment Module. If 'Station Name' is blank the value for Local AE Title shall be used.
3			TEXT	EV (121014,DCM, "Device Observer Manufacturer")	1	U		Defaults to value of Manufacturer (0008,0070) in General Equipment Module
4			TEXT	EV (121015,DCM, "Device Observer Model Name")	1	U		Defaults to value of Manufacturer's Model Name (0008,1090) in General Equipment Module
5			TEXT	EV (121016,DCM, "Device Observer Serial Number")	1	U		Defaults to value of Device Serial Number (0018,1000) in General Equipment Module
6			TEXT	EV (121017,DCM, "Device Observer Physical Location during observation")	1	U		Hospital Name.
7			CODE	EV (113876, DCM, "Device Role in Procedure")	1-n	U		(113859, DCM, "Irradiating Device")

5.7.2 Standard Extended Templates

The Product supports the following extensions or restrictions to standard templates for SOP Instances created by this product. Extensions or restrictions are indicated by **bold text**.

6. MODALITY WORKLIST QUERY IMPLEMENTATION

6.1 INTRODUCTION

This section specifies the use of the DICOM Modality Worklist Information Model used to organize data and against which a Modality Worklist Query will be performed.

6.2 OEC ELITE MINIVIEW MAPPING OF DICOM ENTITIES

The OEC Elite MiniView maps DICOM Information Entities to local Information Entities in the product's database and user interface.

TABLE 6-1
MAPPING OF DICOM ENTITIES TO OEC ELITE MINIVIEW ENTITIES

DICOM	OEC Elite MiniView Entity
Scheduled Procedure Step	Exam
Requested Procedure	Exam
Imaging Service Request	Exam
Visit	Not Applicable
Patient	Patient

6.3 WORKLIST QUERY MODULE TABLE

See DICOM PS 3.3 and PS 3.4 for a complete definition of the entities, modules, and attributes.

TABLE 6-2
MODALITY WORKLIST INFORMATION MODEL MODULES

Entity Name	Module Name	Reference
Scheduled Procedure Step	SOP Common	6.4.1.1
	Scheduled Procedure Step	6.4.1.2
Requested Procedure	Requested Procedure	6.4.2.1
Imaging Service Request	Imaging Service Request	6.4.3.1
Visit	Visit Identification	6.4.4.1
	Visit Status	6.4.4.2
	Visit Relationship	6.4.4.3
	Visit Admission	6.4.4.4
Patient	Patient Relationship	6.4.5.1
	Patient Identification	6.4.5.2
	Patient Demographic	6.4.5.3
	Patient Medical	6.4.5.4

6.4 WORKLIST QUERY MODULE DEFINITIONS

Please refer to DICOM Standard PS 3.3. (Information Object Definitions) for a description of each of the query key attributes contained within the Modality Worklist Information Model.

6.4.1 Common Scheduled Procedure Step Entity Modules

6.4.1.1 SOP Common Module

TABLE 6-3
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into Instance / MPPS	Note
Specific Character Set	(0008,0005)	O	1C	Yes/Yes	See Section 6.4.1.1.1 below

6.4.1.1.1 Specific Character Set

The attribute Specific Character Set (0008,0005) will always be sent.

As a Query SCU, it will similarly accept response items with ISO_IR 100 values of Specific Character Set or empty value of Specific Character Set (absence of (0008,0005) which mean usage of ASCII Chars only).

The product user interface will allow the user to enter characters from the console keyboard that is within ISO 8859-1 characters.

Please also refer to Section 2.7.

TABLE 6-4
SCHEDULED PROCEDURE STEP MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into Instance / MPPS	Note
Scheduled Procedure Step Sequence	(0040,0100)	R	1	No/No	
>Scheduled Station AE Title	(0040,0001)	R	1	No/No	No Matching is performed.
>Scheduled Procedure Step Start Date	(0040,0002)	R	1	No/No	Using the date configured from the DICOM query filter screen, the following matching can be done: YYYY- year, MM- month, DD- day. Range matching can also be done YYYYMMDD-YYYYMMDD - all matches included between those dates. The “dash” is important -YYYYMMDD - all matches prior to and including this date. The beginning “dash” is important. YYYYMMDD- all matches after and including this date. The ending “dash” is important. Single matching where the dates entered is equal. The data entered on the user interface is passed to the Server as entered; if it does not work see the Server DICOM conformance statement.
>Scheduled Procedure Step Start Time	(0040,0003)	R	1	No/No	No Matching is performed.
>Scheduled Procedure Step End Date	(0040,0004)	O	3	No/No	Not Requested
>Scheduled Procedure Step End Time	(0040,0005)	O	3	No/No	Not Requested
>Modality	(0008,0060)	R	1	No/No	Matching is supported and is configured by the user interface. This value could be set to RF/XA/CR/OT/ALL. “ALL” means any modality. Note 1: Send the field as empty to request universal matching when "ALL" is selected from the UI. Note 2: User could only select RF,XA,CR or OT as Modality Type during image archiving.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare
1694829 REV 3

>Scheduled Performing Physician's Name	(0040,0006)	R	2 *	Yes/Yes	Matching is performed. The data entered on the user interface is passed to the server as it is. Single matching is supported for this data element. This value is mapped into (0008, 1050) in the instance. This value is mapped into (0008, 1050) in the MPPS. Supports 5 different components delimited by “^”, 64 bytes maximum per component group.
>Scheduled Procedure Step Description	(0040,0007)	O	1C *	Yes/Yes	No Matching is performed. This value is mapped into (0040,0275)->(0040, 0007) & Protocol Name(0018,1030) & Series Description(0008,103E) in the image instance. This value is mapped into Series Description(0008,103E) & EV(125203, DCM, “Acquisition Protocol”) in the RDSR instance. This value is mapped into (0040,0270)->(0040, 0007) & Protocol Name(0018,1030) & Series Description(0008,103E) in the MPPS.
>Scheduled Station Name	(0040,0010)	O	2	No/No	No Matching is performed.
>Scheduled Procedure Step Location	(0040,0011)	O	2	No/No	No Matching is performed.
>Scheduled Protocol Code Sequence	(0040,0008)	O	1C	Yes/Yes	No Matching is performed. This value is mapped into (0040,0275)-> (0040, 0008) in the instance. This value is mapped into (0040,0270)-> (0040, 0008) in the MPPS.
>>Code Value	(0008,0100)	O	1	Yes/Yes	No Matching is performed.
>>Coding Scheme Designator	(0008,0102)	O	1	Yes/Yes	No Matching is performed.
>>Coding Scheme Version	(0008,0103)	O	3	Yes/Yes	No Matching is performed.
>>Code Meaning	(0008,0104)	O	3 *	Yes/Yes	No Matching is performed.
>Pre-Medication	(0040,0012)	O	2C	No/No	No Matching is performed.
>Scheduled Procedure Step ID	(0040,0009)	O	1 *	Yes/Yes	No Matching is performed. This value is mapped into (0040,0275)-> (0040, 0009) in the instance. This value is mapped into (0040,0270)-> (0040, 0009) in the MPPS.
>Requested Contrast Agent	(0032,1070)	O	2C	Yes/No	No Matching is performed. This value is mapped into (0018, 0010) in the instance.

>Scheduled Procedure Step Status	(0040,0020)	O	3	No/No	Not Requested
>Comments on the Scheduled Procedure Step	(0040,0400)	O	3	No/No	Not Requested

Note: * in the *Expected Return Key Type* column indicates that this information is displayed on screen, if available

6.4.1.2.1 Scheduled Station AE Title

Always empty in the request, and not used or set for matching.

6.4.2 Common Requested Procedure Entity Modules

6.4.2.1 Requested Procedure Module

TABLE 6-5
REQUESTED PROCEDURE MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into Instance / MPPS	Note
Requested Procedure ID	(0040,1001)	O	1 *	Yes/Yes	Matching is performed. The data entered on the user interface is passed to the server as it is. Single matching is supported for this data element. This value is mapped into(0040,0275)->(0040,1001) in the image instance. This value is mapped into (0040,a370)->(0040,1001) in the RDSR. This value is mapped into (0040,0270)->(0040,1001) in the MPPS.
Requested Procedure Description	(0032,1060)	O	1C *	Yes/Yes	This value is mapped into (0040,0275)->(0032,1060) & Study Description(0008,1030) in the image instance. This value is mapped into (0040,A370)->(0032,1060) in the RDSR. This value is mapped into (0040,0270)->(0032,1060) & Study Description(0008,1030) in the MPPS.
Requested Procedure Code Sequence	(0032,1064)	O	1C	Yes/Yes	No Matching is performed. This value is mapped into (0032, 1064) in the image instance. This value is mapped into (0008, 1032) in the MPPS.
>Code Value	(0008,0100)	O	1	Yes/Yes	No Matching is performed.
>Coding Scheme Designator	(0008,0102)	O	1	Yes/Yes	No Matching is performed.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare
1694829 REV 3

>Coding Scheme Version	(0008,0103)	O	3	Yes/Yes	No Matching is performed.
>Code Meaning	(0008,0104)	O	3	Yes/Yes	No Matching is performed.
Study Instance UID	(0020,000D)	O	1	Yes/Yes	The product will adopt the Study Instance UID which is returned in the MWL response. If there is no Study Instance UID returned from MWL server, then new Study Instance UID will be system created.
Study Date	(0008,0020)	O	3	No/No	Not Requested
Study Time	(0008,0030)	O	3	No/No	Not Requested
Referenced Study Sequence	(0008,1110)	O	2	Yes/Yes	This value is mapped into (0008,1110) in the image instance. This value is mapped into (0008,1110) in the RDSR. This value is mapped into (0008, 1110) in the MPPS.
>Referenced SOP Class UID	(0008,1150)	O	1C	Yes/Yes	
>Referenced SOP Instance UID	(0008,1155)	O	1C	Yes/Yes	
Requested Procedure Priority	(0040,1003)	O	2	No/No	No Matching is performed.
Patient Transport Arrangements	(0040,1004)	O	2	No/No	Not Requested
Requested Procedure Location	(0040,1005)	O	3	No/No	Not Requested
Confidentiality Code	(0040,1008)	O	3	No/No	Not Requested
Reporting Priority	(0040,1009)	O	3	No/No	Not Requested
Names of Intended Recipients of Results	(0040,1010)	O	3	No/No	No Matching is performed.
Reason for the Requested Procedure	(0040,1002)	O	3	No/No	No Matching is performed.
Requested Procedure Comments	(0040,1400)	O	3	No/No	Not Requested

Note: * in the *Expected Return Key Type* column indicates that this information is displayed on screen, if available

6.4.2.1.1 Study Instance UID

The product will adopt the Study Instance UID which is returned in the MWL response. If there is no Study Instance UID returned from MWL server, then new Study Instance UID will be created.

GE Healthcare

1694829 REV 3

6.4.3 Common Imaging Service Request Entity Modules

6.4.3.1 Imaging Service Request Module

TABLE 6-6
IMAGING SERVICE REQUEST MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into Instance / MPPS	Note
Accession Number	(0008,0050)	O	2 *	Yes/Yes	Matching is performed. The data entered on the user interface is passed to the server as it is. Single matching is supported for this data element. Truncated to 16 bytes, end truncated This value is mapped into (0008,0050) in the instance or RDSR. This value is mapped into (0008, 0050) in the MPPS.
Requesting Physician	(0032,1032)	O	2	No/No	No Matching is performed. Supports 5 different components delimited by “^”, 64 bytes maximum per component group.
Referring Physician's Name	(0008,0090)	O	2 *	Yes/No	No Matching is performed. This value is mapped into (0008,0090) in the instance or RDSR. Supports 5 different components delimited by “^”, 64 bytes maximum per component group.
Requesting Service	(0032,1033)	O	3	No/No	Not Requested
Reason for the Imaging Service Request	(0040,2001)	O	3	No/No	Not Requested
Imaging Service Request Comments	(0040,2400)	O	3	No/No	Not Requested
Issue Date of Imaging Service Request	(0040,2004)	O	3	No/No	Not Requested
Issue Time of Imaging Service Request	(0040,2005)	O	3	No/No	Not Requested
Placer Order Number / Imaging Service Request	(0040,2016)	O	3	No/No	Not Requested
Filler Order Number / Imaging Service Request	(0040,2017)	O	3	No/No	Not Requested
Order entered by ...	(0040,2008)	O	3	No/No	Not Requested
Order Enterer's Location	(0040,2009)	O	3	No/No	Not Requested
Order Callback Phone Number	(0040,2010)	O	3	No/No	Not Requested

Note: * in the *Expected Return Key Type* column indicates that this information is displayed on screen, if available

6.4.4 Common visit Entity Modules

6.4.4.1 Visit Identification

Not applicable

6.4.4.2 Visit Status

Not applicable

6.4.4.3 Visit Relationship

Not applicable

6.4.4.4 Visit Admission

Not applicable

6.4.5 Common Patient Entity Modules

6.4.5.1 Patient Relationship

Not applicable

6.4.5.2 Patient Identification

TABLE 6-7
PATIENT IDENTIFICATION MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into Instance / MPPS	Note
Patient's Name	(0010,0010)	R	1 *	Yes/Yes	Matching is performed. Single or Wildcard matching is supported for this data element. Supports 5 different components delimited by “^”, 64 bytes maximum per component group.
Patient ID	(0010,0020)	R	1 *	Yes/Yes	Matching is performed. Single matching is supported for this data element. Truncated to 64 bytes, end truncated
Issuer of Patient ID	(0010,0021)	O	3	Yes/Yes	No Matching is performed.
Other Patient IDs	(0010,1000)	O	3	No/No	Not Requested
Other Patient Names	(0010,1001)	O	3	No/No	Not Requested
Patient's Birth Name	(0010,1005)	O	3	No/No	Not Requested

GE Healthcare
1694829 REV 3

Patient's Mother's Birth Name	(0010,1060)	O	3	No/No	Not Requested
Medical Record Locator	(0010,1090)	O	3	No/No	Not Requested

Note: * in the *Expected Return Key Type* column indicates that this information is displayed on screen, if available

6.4.5.3 Patient Demographic

TABLE 6-8
PATIENT DEMOGRAPHIC MODULE ATTRIBUTES

Attribute Name	Tag	Expected Matching Key Type	Expected Returned Key Type	Mapped into Instance / MPPS	Note
Patients Birth Date	(0010,0030)	O	2 *	Yes/Yes	No Matching is performed.. Truncated to 64 bytes, end truncated. If the attribute value is invalid then this value will be set as empty.
Patient's Sex	(0010,0040)	O	2 *	Yes/Yes	No Matching is performed.. Truncated to 2 bytes, end truncated. If the attribute value is invalid then this value will be set as empty.
Patient's Weight	(0010,1030)	O	2*	Yes/No	No Matching is performed.. Only mapped into image instance. Truncated to 16 bytes, end truncated. If the attribute value is invalid then this value will be set as empty.
Confidentiality constraint on patient data	(0040,3001)	O	2	No/No	No Matching is performed.
Patient's Size	(0010,1020)	O	3*	Yes/No	No Matching is performed.. Only mapped into image instance. If the attribute value is invalid then this value will be set as empty. Truncated to 16 bytes, end truncated
Patient's Address	(0010,1040)	O	3	No/No	Not Requested
Patient's Telephone Numbers	(0010,2154)	O	3	No/No	Not Requested
Patient's Age	(0010,1010)	O	3	No/No	Not Requested
Occupation	(0010,2180)	O	3	No/No	Not Requested
Patient's Birth Time	(0010,0032)	O	3	No/No	Not Requested
Patient's Insurance Plan Code Sequence	(0010,0050)	O	3	No/No	Not Requested
> 'Code Sequence Macro'					

**OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT**

GE Healthcare
1694829 REV 3

Patient's Primary Language Code Sequence	(0010,0101)	O	3	No/No	Not Requested
> 'Code Sequence Macro'					
> Patient's Primary Language Code Modifier Sequence	(0010,0102)	O	3	No/No	Not Requested
>> 'Code Sequence Macro'					
Military Rank	(0010,1080)	O	3	No/No	Not Requested
Branch of Service	(0010,1081)	O	3	No/No	Not Requested
Country of Residence	(0010,2150)	O	3	No/No	Not Requested
Region of Residence	(0010,2152)	O	3	No/No	Not Requested
Patient's Telephone Numbers	(0010,2154)	O	3	No/No	Not Requested
Ethnic Group	(0010,2160)	O	3	No/No	Not Requested
Patient's Religious Preference	(0010,21F0)	O	3	No/No	Not Requested
Patient Comments	(0010,4000)	O	3*	Yes/No	No Matching is performed. Mapped into image and RDSR instance . Truncated to 10240 bytes, end truncated

Note: * in the *Expected Return Key Type* column indicates that this information is displayed on screen, if available

6.4.5.4 Patient Medical

Not applicable

7. MODALITY PERFORMED PROCEDURE STEP IMPLEMENTATION

7.1 INTRODUCTION

This section specifies the use of the DICOM Modality Performed Procedure Step information to be communicated to the Hospital/Radiology information system.

This feature works in conjunction with DICOM Modality Worklist feature, if installed. However the conformance of this feature is independent of Modality Worklist feature. For information on conformance of Modality Worklist feature to DICOM standard please refer to the appropriate section in this document.

7.2 RELATIONSHIP BETWEEN SCHEDULED AND PERFORMED PROCEDURE STEPS

OEC Elite MiniView supports following relationship between Scheduled Procedure Step and PPS:

1. Supports a one-to-one relationship between Scheduled Procedure Step and PPS
2. Supports one-to-multiple relationship: Append Case with new PPS based on Original SPS
3. Supports Unscheduled Case or Acquisition without MWL Data

7.3 MODALITY PERFORMED PROCEDURE STEP MODULE TABLE

See DICOM PS 3.3 and PS 3.4 for a complete definition of the entities, modules, and attributes.

TABLE 7-1
MODALITY PERFORMED PROCEDURE STEP MODULES

Module Name	Reference
SOP Common	7.4.1
Performed Procedure Step Relationship	7.4.2
Performed Procedure Step Information	7.4.3
Image Acquisition Results	7.4.4
Radiation Dose	7.4.5
Billing and Material Management Codes	7.4.6

7.4 MODALITY PERFORMED PROCEDURE STEP MODULE DEFINITIONS

Please refer to DICOM Standard PS 3.3. (Information Object Definitions) for a description of each of the attributes contained within the Modality Performed Procedure Step Information Object Definition.

GE Healthcare

1694829 REV 3

7.4.1 SOP Common Module

TABLE 7-2
SOP COMMON MODULE ATTRIBUTES

Attribute Name	Tag	Type for SCU N-CREATE	Type for SCU N-SET	Use
Specific Character Set	(0008,0005)	1C	1C	ISO_IR 100

7.4.2 Performed Procedure Step Relationship Module

TABLE 7-3
PERFORMED PROCEDURE STEP RELATIONSHIP MODULE ATTRIBUTES

Attribute Name	Tag	Type for SCU - N-CREATE	
		Acquisition without MWL Entry	Acquisition with MWL Entry
Scheduled Step Attributes Sequence	(0040,0270)	1, Only 1 item	1, Only 1 item
>Study Instance UID	(0020,000D)	1, System generated.	1, Got from MWL.
>Referenced Study Sequence	(0008,1110)	2, Empty.	2, Got from MWL, Only 1 item.
>>Referenced SOP Class UID	(0008,1150)	1, Not sent	1, Got from MWL.
>>Referenced SOP Instance UID	(0008,1155)	1, Not sent	1, Got from MWL.
>Accession Number	(0008,0050)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
>Placer Order Number/Imaging Service Request	(0040,2016)	3, Not sent	3, Not sent
>Filler Order Number/Imaging Service Request	(0040,2017)	3, Not sent	3, Not sent
>Requested Procedure ID	(0040,1001)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
>Requested Procedure Code Sequence	(0032,1064)	3, Not sent	3, Not sent
>>Code Value	(0008,0100)	1, Not sent	1, Not sent
>>Coding Scheme Designator	(0008,0102)	1, Not sent	1, Not sent
>>Code Meaning	(0008,0104)	1, Not sent	1, Not sent
>Requested Procedure Description	(0032,1060)	2, User input. If user does not provide input values, then empty	2, Got from MWL.

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

>Scheduled Procedure Step ID	(0040,0009)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
>Scheduled Procedure Step Description	(0040,0007)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
>Scheduled Protocol Code Sequence	(0040,0008)	2, empty	2, Got from MWL
>>Code Value	(0008,0100)	1, Not sent	1, Got from MWL
>>Coding Scheme Designator	(0008,0102)	1, Not sent	1, Got from MWL
>>Coding Scheme Version	(0008,0103)	3, Not sent	3, Got from MWL
>>Code Meaning	(0008,0104)	3, Not sent	3, Got from MWL
Patient's Name	(0010,0010)	2, User input. If user does not provide input values, then UNNAMED xxxxx should be assigned to Last Name (xxxxx is a 5-digital number)	2, Got from MWL.
Patient ID	(0010,0020)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
Issuer of Patient ID	(0010,0021)	3, empty	3, Got from MWL.
Patient's Birth Date	(0010,0030)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
Patient's Sex	(0010,0040)	2, User input. If user does not provide input values, then empty	2, Got from MWL.
Referenced Patient Sequence	(0008,1120)	2, empty.	2, empty.
>Referenced SOP Class UID	(0008,1150)	1, Not sent	1, Not sent
>Referenced SOP Instance UID	(0008,1155)	1, Not sent	1, Not sent
Admission ID	(0038,0010)	3, Not sent	3, Not sent
Issuer of Admission ID	(0038,0011)	3, Not sent	3, Not sent
Service Episode ID	(0038,0060)	3, Not sent	3, Not sent
Issuer of Service Episode ID	(0038,0061)	3, Not sent	3, Not sent
Service Episode Description	(0038,0062)	3, Not sent	3, Not sent

7.4.3 Performed Procedure Step Information Module

TABLE 7-4
PERFORMED PROCEDURE STEP INFORMATION MODULE ATTRIBUTES

Attribute Name	Tag	Type for SCU N-CREATE	Type for SCU N-SET	Use
Performed Procedure Step ID	(0040,0253)	1	-	If Scheduled Procedure Step ID is empty then this value is current timestamp, else this value is Scheduled Procedure Step ID.
Performed Station AE Title	(0040,0241)	1	-	Got from configure file.
Performed Station Name	(0040,0242)	2	-	Got from configure file.
Performed Location	(0040,0243)	2	-	Got from configure file. The value is Hospital Name.
Performed Procedure Step Start Date	(0040,0244)	1	-	Same as exam start date
Performed Procedure Step Start Time	(0040,0245)	1	-	Same as exam start time
Performed Procedure Step Status	(0040,0252)	1	3	When PPS start (N-CREATE) message is sent, this element will have the value "IN PROGRESS" . When PPS end (N-SET) message is sent, this element will have either "COMPLETED" or "DISCONTINUED" based on user selection.
Performed Procedure Step Description	(0040,0254)	2	3	This value is Scheduled Procedure Step Description
Performed Procedure Type Description	(0040,0255)	2	3	From "Requested Procedure Description" on screen which is come from MWL.
Procedure Code Sequence	(0008,1032)	2	3	Always set as Empty for local created exam. When using MWL, this value is Requested Procedure Code Sequence.
>Code Value	(0008,0100)	1	1	Only when using MWL sent.
>Coding Scheme Designator	(0008,0102)	1	1	Only when using MWL sent.
>Coding Scheme Version	(0008,0103)	3	3	Only when using MWL sent.
>Code Meaning	(0008,0104)	3	3	Only when using MWL sent.
Performed Procedure Step End Date	(0040,0250)	2	3	Date when PPS end got installed
Performed Procedure Step End Time	(0040,0251)	2	3	Time when PPS end got installed
Comments on the Performed Procedure Step	(0040,0280)	3	3	Not sent
Performed Procedure Step Discontinuation Reason Code Sequence	(0040,0281)	3	3	Used when exam is DISCONTINUED. Provide a way let user to select one
>Code Value	(0008,0100)	1	1	Follow CID 9301
>Coding Scheme Designator	(0008,0102)	1	1	Follow CID 9301

GE Healthcare

1694829 REV 3

>Coding Scheme Version	(0008,0103)	3	3	Follow CID 9301
>Code Meaning	(0008,0104)	3	3	Follow CID 9301

7.4.4 Image Acquisition Results Module

TABLE 7-5
IMAGE ACQUISITION RESULTS MODULE ATTRIBUTES

Attribute Name	Tag	Type for SCU N-CREATE	Type for SCU N-SET	Use
Modality	(0008,0060)	1	-	When user create a local scheduled exam, then this value will be set as "RF" as default. Got from MWL server.
Study ID	(0020,0010)	2	-	System creates and Read Only on screen.
Performed Protocol Code Sequence	(0040,0260)	2	3	Always set as Empty.
>Code Value	(0008,0100)	1	1	Not sent
>Coding Scheme Designator	(0008,0102)	1	1	Not sent
>Coding Scheme Version	(0008,0103)	3	3	Not sent
>Code Meaning	(0008,0104)	3	3	Not sent
Performed Series Sequence	(0040,0340)	2	3	N-Set: Will be sent with referenced instances.
>Performing Physician's Name	(0008,1050)	2	2	Got from MWL server. User input.
>Protocol Name	(0018,1030)	1	1	When using MWL, if Scheduled Protocol Sequence Code Meaning is not empty then this value is Scheduled Protocol Sequence Code Meaning, else this value is Scheduled Procedure Step Description. When using local created exam, if Protocol Description is empty then it will be set as "Unknown Protocol" else it will be Protocol Description.
>Operator's Name	(0008,1070)	2	2	Always set as Empty.
>Series Instance UID	(0020,000E)	1	1	System creates.
>Series Description	(0008,103E)	2	2	This value is Protocol Name.
>Retrieve AE Title	(0008,0054)	2	2	Always set as Empty.
> Archive Requested	(0040,A494)	3	3	Not sent
>Referenced Image Sequence	(0008,1140)	2	2	Will be sent with referenced images. One item for each image created within the series
>>Referenced SOP Class UID	(0008,1150)	1	1	Referenced image SOP Class UID.
>>Referenced SOP Instance UID	(0008,1155)	1	1	Referenced image SOP Instance UID.

GE Healthcare

1694829 REV 3

>Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	2	2	Will be sent with referenced instance
>>Referenced SOP Class UID	(0008,1150)	1	1	Referenced instance SOP Class UID.
>>Referenced SOP Instance UID	(0008,1155)	1	1	Referenced instance SOP instance UID.

7.4.5 Radiation Dose Module

TABLE 7-6
RADIATION DOSE MODULE ATTRIBUTES

Attribute Name	Tag	Type for SCU N-CREATE	Type for SCU N-SET	Use
Anatomic Structure, Space or Region Sequence	(0008,2229)	3	3	Always set as empty.
Total Time of Fluoroscopy	(0040,0300)	3	3	Got value from DB.
Total Number of Exposures	(0040,0301)	3	3	Got value from DB.
Distance Source to Detector (SID)	(0018,1110)	3	3	Got value from configure file.
Distance Source to Entrance	(0040,0306)	3	3	Not sent
Entrance Dose	(0040,0302)	3	3	Got value from DB.
Entrance Dose in mGy	(0040,8302)	3	3	The same with (0040,0302), but unit is mGy.
Exposed Area	(0040,0303)	3	3	Not sent
Image Area Dose Product	(0018,115E)	3	3	Got value from DB.
Comments on Radiation Dose	(0040,0310)	3	3	Not Used
Exposure Dose Sequence	(0040,030E)	3	3	Zero or more items shall be included in this sequence. The items count will be the shot count.
>Radiation Mode	(0018,115A)	3	3	Fixed as "CONTINUOUS"
>KVp	(0018,0060)	3	3	Got value from DB.
>X-ray Tube Current in μ A	(0018,8151)	3	3	Got value from DB.
>Exposure Time	(0018,1150)	3	3	Got value from DB.
>Filter Type	(0018,1160)	3	3	Not sent
>Filter Material	(0018,7050)	3	3	Not sent

GE Healthcare

1694829 REV 3

7.4.6 Billing and Material Management Codes Module

TABLE 7-7
BILLING AND MATERIAL MANAGEMENT CODES MODULE ATTRIBUTES

Attribute Name	Tag	Type for SCU N-CREATE	Type for SCU N-SET	Use
Billing Procedure Step Sequence	(0040,0320)	3	3	Not sent
> 'Code Sequence Macro'	(0020,0010)	3	3	
Film Consumption Sequence	(0040,0321)	3	3	Not sent
>Number of Films	(2100,0170)	3	3	Not sent
>Medium Type	(2000,0030)	3	3	Not sent
>Film Size ID	(2010,0050)	3	3	Not sent
Billing Supplies and Devices Sequence	(0040,0324)	3	3	Not sent
>Billing Item Sequence	(0040,0296)	3	3	Not sent
>> 'Code Sequence Macro'	(0040,0303)	3	3	Not sent
>Quantity Sequence	(0040,0293)	3	3	Not sent
>>Quantity	(0040,0294)	3	3	Not sent
>>Measuring Units Sequence	(0040,0295)	3	3	Not sent
>>> 'Code Sequence Macro'	(0018,115A)	3	3	Not sent

7.5 STANDARD EXTENDED AND PRIVATE DATA ATTRIBUTES

The Product supports the Standard and Private Attributes defined in the following sections in Standard Extended MPPS Instances as Type 3 data elements.

7.5.1 Standard Attributes

The Product supports the following attributes, not specified in the MPPS IOD, in SOP Instances as Type 3 data elements.

TABLE 7-8
STANDARD EXTENDED ATTRIBUTES

Attribute Name	Tag	Use
N/A	N/A	N/A

7.6 STANDARD EXTENDED AND PRIVATE CONTEXT GROUPS

The Product supports coded terminology using Standard Extended, Private, and Configurable Context Groups defined in the following sections.

7.6.1 Standard Extended Context Groups

The Product supports the following extensions to standard Context Groups for SOP Instances created by this product. Extensions are indicated by **bold text**.

GE Healthcare

1694829 REV 3

7.6.1.1 Context ID 9301 Modality PPS Discontinuation Reasons

Context ID 9301
Modality PPS Discontinuation Reasons

Type: Extensible Version: 20090616

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
DCM	110500	Doctor cancelled procedure
DCM	110501	Equipment failure
DCM	110502	Incorrect procedure ordered
DCM	110503	Patient allergic to media/contrast
DCM	110504	Patient died
DCM	110505	Patient refused to continue procedure
DCM	110506	Patient taken for treatment or surgery
DCM	110507	Patient did not arrive
DCM	110508	Patient pregnant
DCM	110509	Change of procedure for correct charging
DCM	110510	Duplicate order
DCM	110511	Nursing unit cancel
DCM	110512	Incorrect side ordered
DCM	110513	Discontinued for unspecified reason
DCM	110514	Incorrect worklist entry selected
DCM	110515	Patient condition prevented continuing
DCM	110516	Equipment change

8. STORAGE COMMITMENT PUSH MODEL IMPLEMENTATION

8.1 STORAGE COMMITMENT PUSH MODEL INFORMATION OBJECT DEFINITION

Please refer to DICOM Part 3 (Information Object Definitions) for a description of each of the attributes contained within the Storage Commitment Information Object.

The Storage Commitment Information Object is used both for N-ACTION Storage Commitment Requests by the SCU and N-EVENT-REPORT Storage Commitment Notifications by the SCP.

8.1.1 STORAGE COMMITMENT MODULE FOR N-ACTION

TABLE 8-1
STORAGE COMMITMENT MODULE FOR N-ACTION

Attribute Name	Tag	SCU Use	SCP Use
Transaction UID	(0008,1195)	Created by equipment, using prefix: 1.2.840.113619.8.403. +MAC+transactionIndicator(70)+TimeStamp_Current MAC: Number string of device MAC address.	Not used
Storage Media File-Set ID	(0088,0130)	Not used	Not used
Storage Media File-Set UID	(0088,0140)	Not used	Not used
Referenced SOP Sequence	(0008,1199)	Images/RDSR instances might be included here.	Not used
>Referenced SOP Class UID	(0008,1150)		Not used
>Referenced SOP Instance UID	(0008,1155)		Not used
>Storage Media File-Set ID	(0088,0130)	Not used	Not used
>Storage Media File-Set UID	(0088,0140)	Not used	Not used

8.1.2 STORAGE COMMITMENT MODULE FOR N-EVENT-REPORT

TABLE 8-2
STORAGE COMMITMENT MODULE FOR N-EVENT-REPORT

Attribute Name	Tag	SCU Use
Transaction UID	(0008,1195)	Value received from SCP, if the value is empty, then return failed.
Retrieve AE Title	(0008,0054)	Not used
Storage Media File-Set ID	(0088,0130)	Not used
Storage Media File-Set UID	(0088,0140)	Not used

Referenced SOP Sequence	(0008,1199)	Success of storage commitment is reported to the user. This sequence will be used to mark storage status on screen. All the succeeded instance will marked as “Stored” in the system.
>Referenced SOP Class UID	(0008,1150)	
>Referenced SOP Instance UID	(0008,1155)	
>Retrieve AE Title	(0008,0054)	Not Used
>Storage Media File-Set ID	(0088,0130)	Not used
>Storage Media File-Set UID	(0088,0140)	Not used
Failed SOP Sequence	(0008,1198)	All the failed instance will not be marked as “Stored” in the system.
>Referenced SOP Class UID	(0008,1150)	
>Referenced SOP Instance UID	(0008,1155)	
>Failure Reason	(0008,1197)	See Section 8.1.2.1 for the list of processed values.

8.1.2.1 Processing of Failure Reason when received in a N-Event-Report

When receiving an N-Event-Report request with an Event Type ID equal to 2, meaning that Storage Commitment is complete, but failure exists, following is the set of value that this Storage Commitment SCU AE is able to process:

Failure Reason	Meaning	Application Behavior When Receiving Reason Code
0110H	Processing failure	Failure and reason is logged. A general failure is reported to the user.
0112H	No such object instance	
0213H	Resource limitation	
0122H	Referenced SOP Class not supported	
0119H	Class / Instance conflict	
0131H	Duplicate transaction UID	
*	Other Failure Reason code values	

9. BASIC DIRECTORY INFORMATION OBJECT IMPLEMENTATION

9.1 IOD MODULE TABLE

Table 9-1 identifies the defined modules within the entities which comprise the Basic Directory IOD. Modules are identified by Module Name.

See DICOM Part 3 for a complete definition of the entities, modules, and attributes.

TABLE 9-1
BASIC DIRECTORY IOD MODULES

Entity Name	Module Name	Reference
File Set Identification	File Set Identification	9.2.1
Directory Information	Directory Information	9.2.2

The FSC of this implementation creates a Directory Information Module for new media and creates XA IOD.

9.2 INFORMATION MODULE DEFINITIONS

Please refer to DICOM Standard Part 3 (Information Object Definitions) for a description of each of the entities and modules contained within the Basic Directory Information Object.

The following modules are included to convey Enumerated Values, Defined Terms, and Optional Attributes supported. Type 1 & Type 2 Attributes are also included for completeness and to define what values they may take and where these values are obtained from. It should be noted that they are the same ones as defined in the DICOM Standard Part 3 (Information Object Definitions). Also note that Attributes not present in tables are not supported.

GE Healthcare

1694829 REV 3

9.2.1 File Set identification Module

TABLE 9-2
FILE-SET IDENTIFICATION MODULE

Attribute Name	Tag	Type	Attribute Description
File-set ID	(0004,1130)	2	Current DateTime stamp, format like:YYYYMMDDHHMMSS YYYY- year, MM- month, DD- day. HH – Hour 00-23, MM – minute 00-59, SS – second 00-59
File-set Descriptor File ID	(0004,1141)	3	Not Used
Specific Character Set of File-set Descriptor File	(0004,1142)	1C	Not Used

9.2.2 Directory Information Module

TABLE 9-3
DIRECTORY INFORMATION MODULE

Attribute Name	Tag	Type	Attribute Description
Offset of the First Directory Record of the Root Directory Entity	(0004,1200)	1	The number of bytes from the beginning of the file to the first byte of the first Directory Record. When the Root Directory entity contains no directory record, this offset is set to 00000000H
Offset of the Last Directory Record of the Root Directory Entity	(0004,1202)	1	The number of bytes from the beginning of the file to the first byte of the last Directory Record. When the Root Directory entity contains no directory record, this offset is set to 00000000H
File-set Consistency Flag	(0004,1212)	1	FSC writes 0000H: no known inconsistencies.
Directory Record Sequence	(0004,1220)	2	FSC creates items in this sequence (Directory Records).
>Offset of the Next Directory Record	(0004,1400)	1C	
>Record In-use Flag	(0004,1410)	1C	Set the value to 0xFFFF for record is in use
>Offset of Referenced Lower-Level Directory Entity	(0004,1420)	1C	
>Directory Record Type	(0004,1430)	1C	Enumerated Values are created by an FSC/FSU: PATIENT STUDY SERIES IMAGE SR DOCUMENT
>Private Record UID	(0004,1432)	1C	Not Used
>Referenced File ID	(0004,1500)	1C	Filename is generated to be unique on the media like: DCM<index>\IMG<number of image> Field is included if Directory Record Type is not PATIENT/STUDY/SERIES.

>Referenced SOP Class UID in File	(0004,1510)	1C	Field is included if Directory Record Type is not PATIENT/STUDY/SERIES. Unique ID for the SOP Class of the Instance stored in the referenced File.
>Referenced SOP Instance UID in File	(0004,1511)	1C	Field is included if Directory Record Type is not PATIENT/STUDY/SERIES. Unique Identifier for the SOP Instance stored in the referenced file.
>Referenced Transfer Syntax UID in File	(0004,1512)	1C	Field is included if Directory Record Type is not PATIENT/STUDY/SERIES. Unique Identifier for the Transfer Syntax used to encode the Instance stored in the referenced file.
> Referenced Related General SOP Class UID in File	(0004,151A)	1C	Not Used
>Record Selection Keys			See 9.2.3

9.2.3 Definition of Specific Directory Records

9.2.3.1 Patient Directory Record Definition

TABLE 9-4
PATIENT KEYS

Key	Tag	Type	Attribute Description
Specific Character Set	(0008,0005)	1C	ISO_IR 100
Patient's Name	(0010,0010)	2	FSC/FSU will fill this attribute with the value in the referenced composite object instance.
Patient ID	(0010,0020)	1	FSC/FSU will fill this attribute with the value in the referenced composite object instance. FSC/FSU will fill this mandatory attribute with a value "DCMTKPAT + 6 digits" if it is empty in the referenced composite object instance.

9.2.3.2 Study Directory Record Definition

TABLE 9-5
STUDY KEYS

Key	Tag	Type	Attribute Description
Specific Character Set	(0008,0005)	1C	ISO_IR 100
Study Date	(0008,0020)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance. This value is mandatory for OEC Elite MiniView, can't be empty.
Study Time	(0008,0030)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance. This value is mandatory for OEC Elite MiniView, can't be empty.

Study Description	(0008,1030)	2	FSC/FSU will fill this attribute with the value in the referenced composite object instance.
Study Instance UID	(0020,000D)	1C	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance. This value is mandatory for OEC Elite MiniView, can't be empty.
Study ID	(0020,0010)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance. FSC/FSU will fill this mandatory attribute with a value "DCMTKSTUDY+ 6 digits" if it is empty in the referenced composite object instance.
Accession Number	(0008,0050)	2	FSC/FSU will fill this attribute using the value in the referenced composite object instance.

9.2.3.3 Series Directory Record Definition

TABLE 9-6
SERIES KEYS

Key	Tag	Type	Attribute Description
Specific Character Set	(0008,0005)	1C	ISO_IR 100
Modality	(0008,0060)	1	This will be consistent with Image Content
Series Instance UID	(0020,000E)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance. This value is mandatory for OEC Elite MiniView, can't be empty.
Series Number	(0020,0011)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance. FSC/FSU will fill this mandatory attribute with a value start from 1 (+1 for each series) if it is empty in the referenced composite object instance.
Icon Image Sequence	(0088,0200)	3	Not Used
>Include 'Image Pixel Macro'			See 9.2.3.3.1

9.2.3.3.1 Icon Image Key Definition

Not applicable

9.2.3.4 Image Directory Record Definition

TABLE 9-7
IMAGE KEYS

Key	Tag	Type	Attribute Description
Specific Character Set	(0008,0005)	1C	ISO_IR 100
Image Type	(0008,0008)	3	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance.
Instance Number	(0020,0013)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance.
Icon Image Sequence	(0088,0200)	3	FSC/FSU will create Icon Images at the image level.
>Include 'Image Pixel Macro'			See section 9.2.3.4.1

- Note: Please also refer to Section 3.2.1.2.1.1.1 for information about Additional Keys sent in DICOMDIR.

9.2.3.4.1 Icon Image Key Definition

- The FSC creates the icon image sequence from the referenced composite object instance. The FSR displays image icons to the user without reading the actual image pixel from the media.
- Samples Per pixel (0028,0002) is set to 1.
- Photometric Interpretations (0028,0004) is set to MONOCHROME2.
- Row (0028,0010) and Column (0028,0011) are set to 128,128.
- Bits Allocated (0028,0100) and Bits Stored (0028,0101) are created and set to 8.
- High Bit (0028,0102) is created and set to 7.
- Pixel Representation (0028,0103) is created and set to 0.

Pixel Data (7EF0,0010) is set with the 128x128 icon image data.

9.2.3.5 SR Document Directory Record Definition

TABLE 9-8
SR DOCUMENT KEYS

Key	Tag	Type	Attribute Description
Specific Character Set	(0008,0005)	1C	ISO_IR 100
Instance Number	(0020,0013)	1	FSC/FSU will fill this mandatory attribute with the value in the referenced composite object instance.
Completion Flag	(0040,A491)	1	"COMPLETE"
Verification Flag	(0040,A493)	1	"Unverified".
Content Date	(0008,0023)	1	First Shot Date
Content Time	(0008,0033)	1	First Shot Time
Verification DateTime	(0040,A030)	1C	Not Used
Concept Name Code Sequence	(0040,A043)	1	One item shall be included in this sequence.
>Code Value	(0008,0100)	1	"113701"
>Coding Scheme Designator	(0008,0102)	1	"DCM"
>Code Meaning	(0008,0104)	1	"X-Ray Radiation Dose Report"
Content Sequence	(0040,A730)	1C	
>Relationship Type	(0040,A010)	1	All, and only, Content Items with the HAS CONCEPT MOD relationship from the root Content Item shall be included in this Sequence.
>Include 'Document Content Macro'			

9.3 PRIVATE DATA DICTIONARY

Not applicable.

10. PRINT MANAGEMENT IMPLEMENTATION

10.1 INTRODUCTION

This section of the DICOM Conformance Statement specifies the implementation for the specific SOP Classes supported in the Basic Grayscale Print Management Meta SOP Class, the attributes supported for both IODs and services, and the valid range of values for mandatory and optional attributes.

10.2 BASIC FILM SESSION SOP CLASS

10.2.1 Basic Film Session N-Create Attributes

This table lists the attributes that are sent in the Basic Film Session N-Create Request:

Attribute name	Tag	Use
Specific Character Set	(0008,0005)	Not Used
Number of Copies	(2000,0010)	Range of this value is 1-10, default is 1.
Print Priority	(2000,0020)	Enumerated Terms can be sent: HIGH or MED or LOW
Medium Type	(2000,0030)	Enumerated Terms can be sent: PAPER, CLEAR FILM, BLUE FILM, MAMMO CLEAR FILM, MAMMO BLUE FILM
Film Destination	(2000,0040)	Enumerated Terms can be sent: MAGAZINE or PROCESSOR
Film Session Label	(2000,0050)	Set to "GEHC OEC Print SCU"
Memory Allocation	(2000,0060)	Not Used
Owner ID	(2100,0160)	Set to "GEHC OEC"

10.2.2 Basic Film Session N-Delete

The N-DELETE is used to delete the complete Basic Film Session SOP Instance hierarchy. As a result, all references to Image SOP Instances within the film session are deleted.

10.3 BASIC FILM BOX SOP CLASS

10.3.1 Basic Film Box N-Create Attributes

This table lists the attributes that are sent to the SCP in the Basic Film Box N-Create Request, and that are received in the Basic Film Box N-Create Response from the SCP

Attribute Name	Tag	Use
Image Display Format	(2010,0010)	User configurable. User values =: STANDARD\1,1 STANDARD\1,2 STANDARD\2,1 STANDARD\2,2 STANDARD\2,3 STANDARD\3,3 STANDARD\3,4 STANDARD\4,4 STANDARD\4,5 STANDARD\5,4 Default value: First selection when declaring printer.
Referenced Film Session Sequence	(2010,0500)	Used
>Referenced SOP Class UID	(0008,1150)	Set to 1.2.840.10008.5.1.1.1
>Referenced SOP Instance UID	(0008,1155)	This value should be returned from SCP in N-CREATE-RSP Basic Film Session SOP Class; Then this value is sent to SCP in N-CREATE-RQ Basic Film Box SOP Class requesting for Basic Grayscale Image Box SOP Class Instance UID which contained in Referenced Image Box Sequence from SCP.
Referenced Image Box Sequence	(2010,0510)	Used
>Referenced SOP Class UID	(0008,1150)	Set to 1.2.840.10008.5.1.1.4
>Referenced SOP Instance UID	(0008,1155)	Received in the N-Create Response from SCP, this value should be sent to SCP in N-SET-RQ Basic Grayscale Image Box SOP Class
Referenced Basic Annotation Box Sequence	(2010,0520)	Not Used
>Referenced SOP Class UID	(0008,1150)	Not Used
>Referenced SOP Instance UID	(0008,1155)	Not Used
Film Orientation	(2010,0040)	Enumerated Terms can be sent: PORTRAIT or LANDSCAPE
Film Size ID	(2010,0050)	Enumerated Terms can be sent: 8INX10IN 10INX12IN 10INX14IN 11INX14IN 14INX14IN 14INX17IN 24CMX24CM 24CMX30CM
Magnification Type	(2010,0060)	Set to BILINEAR
Max Density	(2010,0130)	User configurable. The default is 300

GE Healthcare
1694829 REV 3

Configuration Information	(2010,0150)	User configurable. This value specifies the DICOM printer parameters. It is defined in the DICOM Printer's Conformance Statement file.
Referenced Presentation LUT Sequence	(2050,0500)	Not Used
>Referenced SOP Class UID	(0008,1150)	Not Used
>Referenced SOP Instance UID	(0008,1155)	Not Used
Annotation Display Format ID	(2010,0030)	Not Used
Smoothing Type	(2010,0080)	Not Used
Border Density	(2010,0100)	Enumerated Terms can be sent: BLACK or WHITE
Empty Image Density	(2010,0110)	Enumerated Terms can be sent: BLACK or WHITE
Min Density	(2010,0120)	User configurable. The default is 20
Trim	(2010,0140)	Set to NO
Illumination	(2010,015E)	Not Used
Reflected Ambient Light	(2010,0160)	Not Used
Requested Resolution ID	(2020,0050)	Not Used
ICC Profile	(0028,2000)	Not Used

10.3.2 Basic Film Box N-Action Attributes

Following are the Action Reply arguments that are supported if present in the N-Action response of the Basic Film Box SOP Class

Action Type Name	Action Type ID	Attribute	Tag	Usage SCU
Print	1	Referenced Print Job Sequence	(2100,0500)	Not Used
		>Referenced SOP Class UID	(0008,1150)	Not Used
		>Referenced SOP Instance UID	(0008,1155)	Not Used
		>Print Job ID	(2100,0010)	Not Used

10.3.3 Basic Film Box N-Delete

The N-DELETE is used to delete the last created Basic Film Box SOP Instance hierarchy. As a result all the information describing the last film is deleted.

10.4 BASIC GRAYSCALE IMAGE BOX SOP CLASS

10.4.1 Basic Grayscale Image Box Pixel N-Set Attributes

This table lists the attributes that are sent in the Basic Grayscale Image Box N-Set Request:

Attribute Name	Tag	Use
Image Position	(2020,0010)	Based on Image Display Format (2010,0010), range of values sent is [1 ~ 20].
Basic Grayscale Image Sequence	(2020,0110)	A sequence which provides the content of the grayscale image pixel data to be printed
>Samples Per Pixel	(0028,0002)	1
>Photometric Interpretation	(0028,0004)	MONOCHROME2
>Rows	(0028,0010)	Value is 1000 Note: For dose summary snapshot, this value will be 1024.
>Columns	(0028,0011)	Value is 1000 Note: For dose summary snapshot, this value will be 980.
>Pixel Aspect Ratio	(0028,0034)	Not Used
>Bits Allocated	(0028,0100)	Value is 16
>Bits Stored	(0028,0101)	Value is 12
>High Bit	(0028,0102)	Value is 11
>Pixel Representation	(0028,0103)	0
>Pixel Data	(7FE0,0010)	Image Pixels
Polarity	(2020,0020)	Not Used
Magnification Type	(2010,0060)	Not Used
Smoothing Type	(2010,0080)	Not Used
Min Density	(2010,0120)	Not Used
Max Density	(2010,0130)	Not Used
Configuration Information	(2010,0150)	Not Used
Requested Image Size	(2020,0030)	Not Used
Requested Decimate/Crop Behavior	(2020,0040)	Not Used
Referenced Presentation LUT Sequence	(2050,0500)	Not Used
> Referenced SOP Class UID	(0008,1150)	Not Used
> Referenced SOP Instance UID	(0008,1155)	Not Used

10.5 PRINTER SOP CLASS

10.5.1 Printer N-Event-Report Attributes

The following table describes the product behavior when receiving an **N-Event-Report** request from the Printer SCP depending on the Event Type ID value.

GE Healthcare
1694829 REV 3

Event Type Name	Event Type ID	Attribute	Tag	Use
Normal	1			Ignored
Warning	2	Printer Status Info	(2110,0020)	Ignored
		Film Destination	(2000,0040)	Ignored
		Printer Name	(2110,0030)	Ignored
Failure	3	Printer Status Info	(2110,0020)	Ignored
		Film Destination	(2000,0040)	Ignored
		Printer Name	(2110,0030)	Ignored

10.5.2 Printer N-Get Attributes

Attribute Name	Tag	Use
Printer Status	(2110,0010)	When status is FAILURE, we'll not execute print any more and inform user print fail and the printer status is abnormal
Printer Status Info	(2110,0020)	Ignored
Printer Name	(2110,0030)	Ignored
Manufacturer	(0008,0070)	Ignored
Manufacturer Model Name	(0008,1090)	Ignored
Device Serial Number	(0018,1000)	Ignored
Software Versions	(0018,1020)	Ignored
Date Of Last Calibration	(0018,1200)	Ignored
Time Of Last Calibration	(0018,1201)	Ignored

11. QUERY IMPLEMENTATION

11.1 OEC ELITE MINIVIEW MAPPING OF DICOM ENTITIES

The OEC Elite MiniView maps DICOM Information Entities to local Information Entities in the product's database and user interface.

TABLE 11-1
MAPPING OF DICOM ENTITIES TO OEC ELITE MINIVIEW ENTITIES

DICOM	OEC Elite MiniView Entity
Patient	Exam
Study	Exam
Series	Exam
Image	Image

11.2 INFORMATION MODEL KEYS

Please refer to DICOM Standard PS 3.4 (Service Class Specifications) for a description of each of the levels contained within the Query/Retrieve Information Model.

11.2.1 Common Query Keys

The query key attributes specified in this section are used at all levels and in all classes of query.

TABLE 11-2
Q/R PATIENT LEVEL COMMON RETRIEVE ATTRIBUTES

Attribute Name	Tag	Type	SCU Use
Specific Character Set	(0008,0005)	-	See 11.2.1.1.1
Query Retrieve Level	(0008,0052)	-	Set to level of query: PATIENT STUDY SERIES IMAGE
Retrieve AE Title	(0008,0054)	-	Returned value will be used for Retrieve AE Title of retrieval of query response item.
Storage Media File-set ID	(0088,0130)	-	Attribute is not requested.
Storage Media File-set UID	(0088,0140)	-	Attribute is not requested.

11.2.1.1 Q/R Common Attribute Descriptions

11.2.1.1.1 Specific Character Set

In Query requests the character set tag (0008,0005) is set to "ISO_IR 100" for all requests.

In processing of query responses the character set tag (0008,0005) is checked: absence of the tag is defined as ISO_IR 6 (7 bit ASCII) or the tag is present ISO_IR 100 (ISO-8859-1 Latin 1) will be accepted.

11.2.2 Patient Level

This section defines the keys at the Patient Level of the Patient Root Query/Retrieve Information Models that are supported by this implementation.

TABLE 11-3
PATIENT LEVEL ATTRIBUTES FOR THE PATIENT ROOT
QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	SCU Use
Patient's Name	(0010,0010)	R*	Single value and wildcard matching are supported. User could enter anything (including wildcard) except "^", "=", and "\". The value entered by the user will be used as matching key, but the response from server depends on server's capability. During the DICOM archive/sending, the "^" and "=" will be used as delimiter (added by system) in Patient Name components.
Patient ID	(0010,0020)	U*	Single value and wildcard matching are supported. User could enter anything (including wildcard) except "\". The value entered by the user will be used as matching key, but the response from server depends on server's capability.
Referenced Patient Sequence	(0008,1120)	O	Not Requested
>Referenced SOP Class UID	(0008,1150)	O	Not Requested
>Referenced SOP Instance UID	(0008,1155)	O	Not Requested
Patient's Birth Date	(0010,0030)	O	Universal Matching
Patient's Birth Time	(0010,0032)	O	Not Requested
Patient's Sex	(0010,0040)	O	Universal Matching
Other Patient IDs	(0010,1000)	O	Not Requested
Other Patient Names	(0010,1001)	O	Not Requested
Ethnic Group	(0010,2160)	O	Not Requested
Patient Comments	(0010,4000)	O	Not Requested

GE Healthcare
1694829 REV 3

Number of Patient Related Studies	(0020,1200)	O	Universal Matching
Number of Patient Related Series	(0020,1202)	O	Universal Matching
Number of Patient Related Instances	(0020,1204)	O	Universal Matching

Note: * in the *Type* column indicates that this information is displayed on screen, if available

11.2.3 Study Level – Patient Root

This section defines the keys at the Study Level of the Patient Root Query/Retrieve Information Models that are supported by this implementation.

TABLE 11-4
STUDY LEVEL ATTRIBUTES FOR THE PATIENT ROOT
QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	SCU Use
Study Date	(0008,0020)	R*	Range value matching is supported. User could select one of "All", "Today", "Since Yesterday", "Last 3 days", "Last 7 days" and "Last 30 days" from the screen, and then date information will be sent as "yyyymmdd-yyyymmdd" format to the server for matching.
Study Time	(0008,0030)	R*	Universal Matching
Accession Number	(0008,0050)	R*	Single value and wildcard matching are supported. Leading and trailing wildcard matching for value entered. The value entered by the user will be used as matching key.
Study ID	(0020,0010)	R	Universal Matching
Study Instance UID	(0020,000D)	U	Universal Matching
Modalities in Study	(0008,0061)	O	Universal Matching
SOP Classes in Study	(0008,0062)	O	Not Requested
Referring Physician's Name	(0008,0090)	O	Universal Matching
Study Description	(0008,1030)	O*	Universal Matching
Procedure Code Sequence	(0008,1032)	O	Not Requested
>Code Value	(0008,0100)	O*	Not Requested
>Coding Scheme Designator	(0008,0102)	O	Not Requested
>Coding Scheme Version	(0008,0103)	O	Not Requested
>Code Meaning	(0008,0104)	O	Not Requested
Name of Physician(s) Reading Study	(0008,1060)	O	Universal Matching

Admitting Diagnoses Description	(0008,1080)	O	Not Requested
Referenced Study Sequence	(0008,1110)	O	Not Requested
>Referenced SOP Class UID	(0008,1150)	O	Not Requested
>Referenced SOP Instance UID	(0008,1155)	O	Not Requested
Issuer of Patient ID	(0010,0021)	O	Not Requested
Patient's Age	(0010,1010)	O	Not Requested
Patient's Size	(0010,1020)	O	Not Requested
Patient's Weight	(0010,1030)	O	Not Requested
Occupation	(0010,2180)	O	Not Requested
Additional Patient History	(0010,21B0)	O	Not Requested
Other Study Numbers	(0020,1070)	O	Not Requested
Number of Study Related Series	(0020,1206)	O	Universal Matching
Number of Study related Instances	(0020,1208)	O	Universal Matching
Interpretation Author	(4008,010C)	O	Not Requested

Note: * in the *Type* column indicates that this information is displayed on screen, if available

11.2.4 Study Level – Study Root

This section defines the keys at the Study Level of the Study Root Query/Retrieve Information Model that are supported by this implementation.

TABLE 11-5
STUDY LEVEL ATTRIBUTES FOR THE STUDY ROOT
QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	SCU Use
Study Date	(0008,0020)	R*	Range value matching is supported. User could select one of "All", "Today", "Since Yesterday", "Last 3 days", "Last 7 days" and "Last 30 days" from the screen, and then date information will be sent as "yyyymmdd-yyyymmdd" format to the server for matching.
Study Time	(0008,0030)	R*	Universal Matching
Accession Number	(0008,0050)	R*	Single value and wildcard matching are supported. The value entered by the user will be used as matching key.
Study ID	(0020,0010)	R	Universal Matching

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare
1694829 REV 3

Patient's Name	(0010,0010)	R*	Single value and wildcard matching are supported. User could enter anything (including wildcard) except "^", "=", and "\". The value entered by the user will be used as matching key, but the response from server depends on server's capability. During the DICOM archive/sending, the "^" and "=" will be used as delimiter (added by system) in Patient Name components.
Patient ID	(0010,0020)	R*	Single value and wildcard matching are supported. User could enter anything (including wildcard) except "\". The value entered by the user will be used as matching key, but the response from server depends on server's capability.
Study Instance UID	(0020,000D)	U	Universal Matching
Modalities in Study	(0008,0061)	O	Universal Matching
SOP Classes in Study	(0008,0062)	O	Not Requested
Referring Physician's Name	(0008,0090)	O	Universal Matching
Study Description	(0008,1030)	O*	Universal Matching
Procedure Code Sequence	(0008,1032)	O	Not Requested
>Code Value	(0008,0100)	O	Not Requested
>Coding Scheme Designator	(0008,0102)	O	Not Requested
>Coding Scheme Version	(0008,0103)	O	Not Requested
>Code Meaning	(0008,0104)	O	Not Requested
Name of Physician(s) Reading Study	(0008,1060)	O	Universal Matching
Admitting Diagnoses Description	(0008,1080)	O	Not Requested
Referenced Study Sequence	(0008,1110)	O	Not Requested
>Referenced SOP Class UID	(0008,1150)	O	Not Requested
>Referenced SOP Instance UID	(0008,1155)	O	Not Requested
Issuer of Patient ID	(0010,0021)	O	Not Requested
Patient's Age	(0010,1010)	O	Not Requested
Patient's Size	(0010,1020)	O	Not Requested
Patient's Weight	(0010,1030)	O	Not Requested
Occupation	(0010,2180)	O	Not Requested
Additional Patient History	(0010,21B0)	O	Not Requested
Other Study Numbers	(0020,1070)	O	Not Requested

Number of Study Related Series	(0020,1206)	O	Universal Matching
Number of Study related Instances	(0020,1208)	O	Universal Matching
Interpretation Author	(4008,010C)	O	Not Requested
Referenced Patient Sequence	(0008,1120)	O	Not Requested
>Referenced SOP Class UID	(0008,1150)	O	Not Requested
>Referenced SOP Instance UID	(0008,1155)	O	Not Requested
Patient's Birth Date	(0010,0030)	O	Universal Matching
Patient's Birth Time	(0010,0032)	O	Not Requested
Patient's Sex	(0010,0040)	O	Universal Matching
Other Patient IDs	(0010,1000)	O	Not Requested
Other Patient Names	(0010,1001)	O	Not Requested
Ethnic Group	(0010,2160)	O	Not Requested
Patient Comments	(0010,4000)	O	Not Requested
Number of Patient Related Studies	(0020,1200)	O	Not Requested
Number of Patient Related Series	(0020,1202)	O	Not Requested
Number of Patient Related Instances	(0020,1204)	O	Not Requested

Note: * in the *Type* column indicates that this information is displayed on screen, if available

11.2.5 Series Level

This section defines the keys at the Series Level of the Patient Root and Study Root Query/Retrieve Information Models that are supported by this implementation.

TABLE 11-6
SERIES LEVEL ATTRIBUTES FOR THE
QUERY/RETRIEVE INFORMATION MODEL

Attribute Name	Tag	Type	SCU Use
Modality	(0008,0060)	R*	Single value matching is supported. User could select one of "XA", "RF", "CR", "SC" and "ALL" for Modality Type from screen, then the corresponding string "XA", "RF", "CR", "OT" and "" will be sent to server for matching. Note: "ALL" means ignore the Modality Type, the Modality Type will leave empty during sending.
Series Number	(0020,0011)	R	Universal Matching
Series Instance UID	(0020,000E)	U	Universal Matching

OEC ELITE MINIVIEW SOFTWARE RELEASE WORKSTATION-1.X
DICOM CONFORMANCE STATEMENT

GE Healthcare

1694829 REV 3

Number of Series Related Instances	(0020,1209)	O	Universal Matching
Series Description	(0008,103E)	O	Universal Matching
Performed Procedure Step ID	(0040, 0253)	O	Not Requested
Referenced Performed Procedure Step Sequence	(0008,1111)	O	Not Requested
>Referenced SOP Class UID	(0008,1150)	O	Not Requested
>Referenced SOP Instance UID	(0008,1155)	O	Not Requested
Request Attribute Sequence	(0040, 0275)	O	Not Requested
>Requested Procedure ID	(0040,1001)	O	Not Requested
>Scheduled Procedure Step ID	(0040,0009)	O	Not Requested
Performed Procedure Step Start Date	(0040,0244)	O	Not Requested
Performed Procedure Step Start Time	(0040,0245)	O	Not Requested

Note: * in the *Type* column indicates that this information is displayed on screen, if available

11.2.6 Image Level

Currently no Image level query requests are made.