



When their ports are
protected, so is your
peace of mind

3M™ Curos™ Disinfecting Port Protectors

CLABSI

is a serious threat

Every I.V. catheter presents potential for central line-associated bloodstream infections (CLABSI).



Up to

1 in 4 patients

who contract CLABSI die.¹

Even when not fatal, CLABSIs can progress to other serious conditions, which can lead to extended hospital stays.²


71,900

preventable central line infections annually.³

1 www.vdh.virginia.gov/epidemiology/surveillance/hai/documents/pdf/CDC_VitalSignsReportMarch2011.pdf

2 Maki DG, Kluger DM, Crnich CJ. The risk of bloodstream infection in adults with different intravascular devices: a systematic review of 200 published prospective studies. *Mayo Clin Proc.* 2006;81(9):1159-1171

3 Mermel LA. Prevention of Intravascular Catheter-Related Infections. *Ann Intern Med.* 2000; 132:391-402.

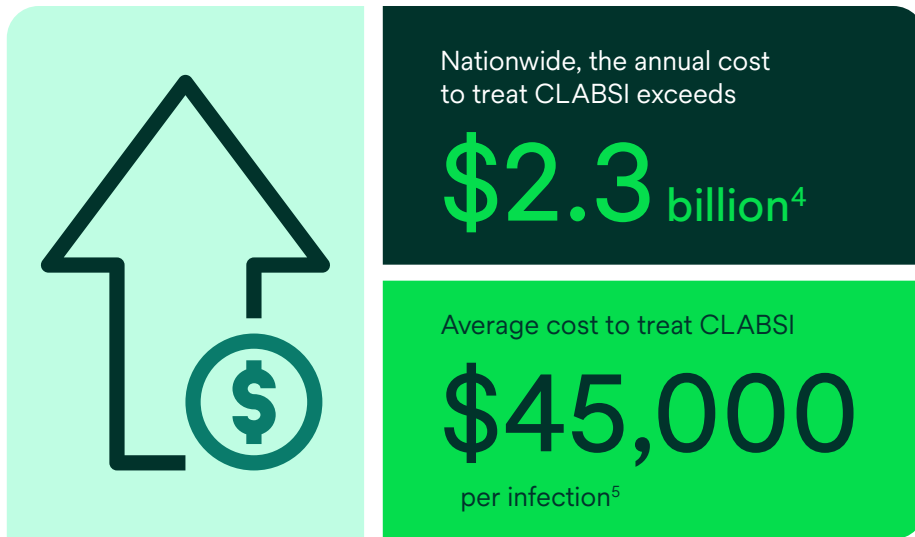

Are all of your ports protected?

This is a picture of a culture taken from an unprotected port. Unprotected ports can touch floors, armpits, bed linens and other unsterile surfaces, adding to their bioburden.⁶




4 Provonost P, Needham D, Berenholtz S, et al. An intervention to decrease catheter-related bloodstream infections in the ICU. *N Engl J Med.* 2006; 355(26): 2725.

5 Zimlichman, E; Henderson, D et al. Health Care–Associated Infections: A Meta-analysis of Costs and Financial Impact on the US Health Care System. *JAMA Intern Med.* Published online September 02, 2013

6 Kaler, W. Making it easy for nurses to reduce the risk of CLABSI, Patient Safety, and Quality Healthcare. 2014; 11 (6), 46-49.

After implementing
Curos disinfecting caps
in one hospital, the rate
of CLABSI decreased
by more than

40%⁷

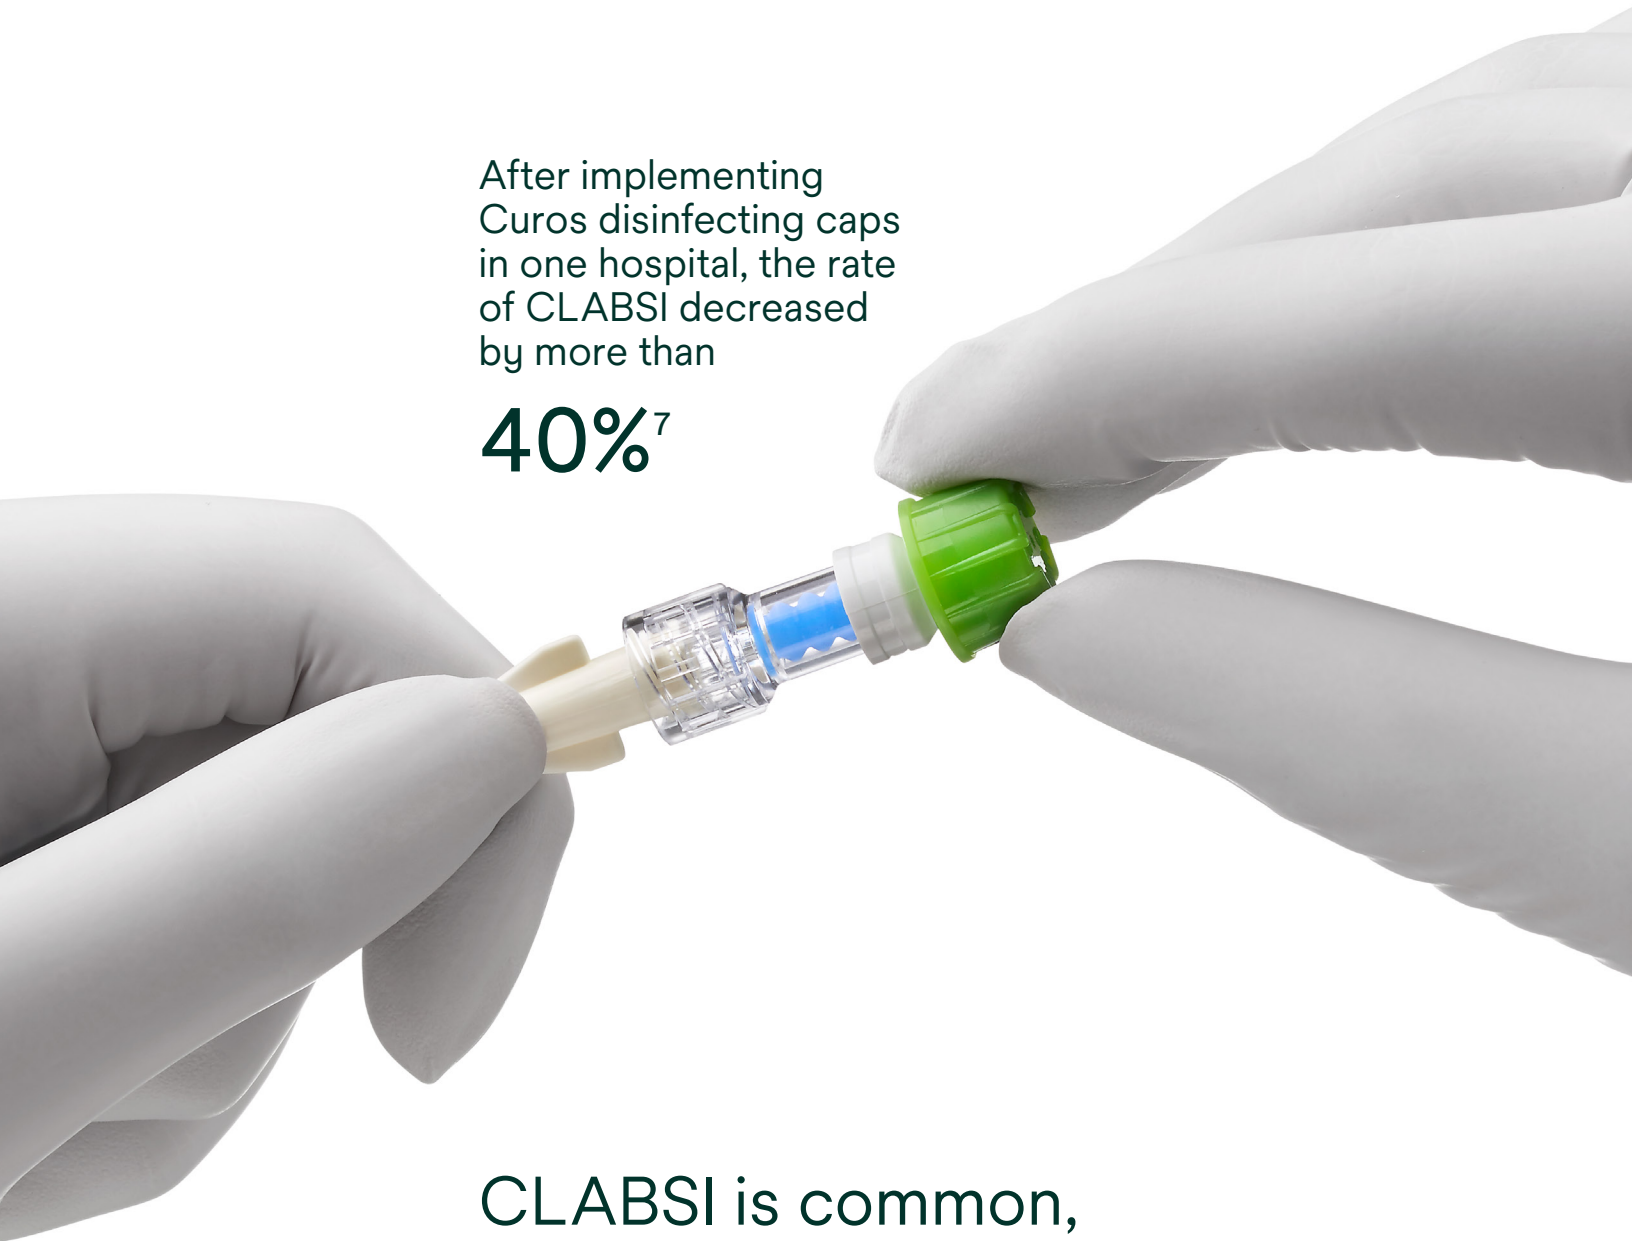

CLABSI is common, but it doesn't have to be.


Consistent use of Curos disinfecting caps on ports is associated with decreased CLABSI. Curos disinfecting port protectors are alcohol-impregnated caps that twist onto ports for disinfection and protection. They disinfect prior to line access and act as a physical barrier to contamination between accesses.

Each Curos disinfecting port protector contains 70% isopropyl alcohol (IPA). The IPA bathes the surface of the port and disinfects it in 1 minute.


⁷ Merrill KC, Sumner S, Linford L, Taylor C, and Macintosh C. Impact of universal disinfectant cap implementation on central line-associated bloodstream infections. American Journal of Infection Control 42 (2014) 1274-7.

3M™ Curoso™ Disinfecting Port Protectors achieved a 99.99% reduction in 6 microbes commonly associated with CLABSI^{8,9}

The effectiveness of Curoso products was tested *in vitro* against⁸:

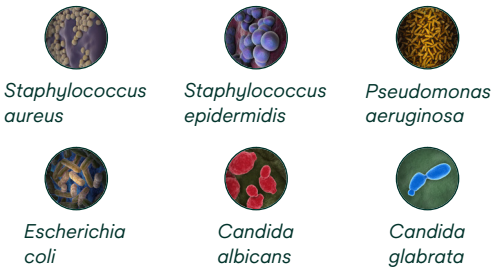

Study conclusion:
All test samples exceeded the minimum 4-log reduction after one minute.
3M data on file.

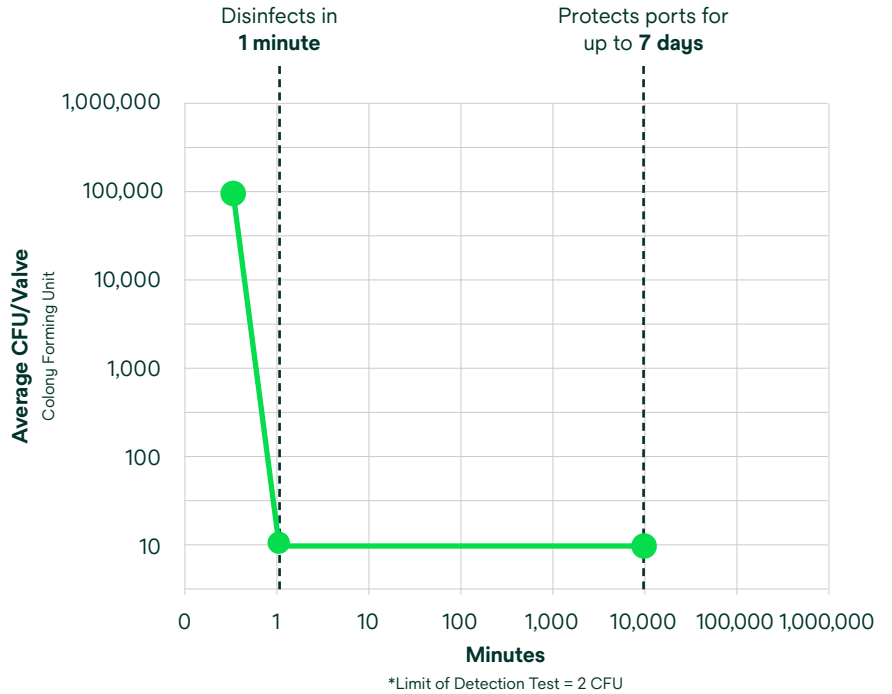

? How do Curoso disinfecting port protectors compare with the “scrub the hub” method?

For more than a decade, the standard of care in port disinfection has been a thorough 15–30 second (plus drying time) manual scrub of the port with an alcohol pad, often referred to as scrubbing the hub. Curoso disinfecting port protectors provide several advantages over the scrub the hub protocol.

A U.S. Hospital observational study showed less than 10% compliance with the disinfection protocol for catheter hubs.¹⁰

- 1 Save time**
Curoso alcohol-impregnated caps provide fast passive disinfection, saving nurses valuable time compared to most scrub the hub protocols. In addition, no drying time is required to achieve disinfection.
- 2 Provide a physical barrier**
They provide a physical barrier to contamination between accesses, for up to 7 days.
- 3 Remove user technique variation**
They remove the user technique variation found in manual scrubbing the hub procedure.
- 4 Provide visual compliance confirmation**
Their bright color also provides quick visual confirmation that a port is clean, giving nurses peace of mind and empowering facilities to audit and improve disinfection compliance.

⁸ Data reflects *in vitro* findings on Curoso™ Disinfecting Port Protectors conducted by an independent laboratory
⁹ For more information regarding organisms associated with catheter-related bloodstream infections, refer to Wenzel RP and Edmond MB. The Impact of Hospital-Acquired Bloodstream Infections. Emerg Infect Dis. 2001 Mar Apr;7(2):174-7.
¹⁰ J. Lee, “Disinfecting cap makes critical difference in central line bundle for reducing CLABSI,” in Proceedings of the APIC Annual Conference vol. 39, p. E64. Fort Lauderdale, Fla, USA, 2013.

When their ports are protected, so is your peace of mind

All patients, all access points, all the time

Use the entire family of 3M™
Curoso Disinfecting Port Protectors
products to reduce risks across
intraluminal access points.



According to the 2016
Infusion Nurses Society
Standards of Practice, “Use
of passive disinfecting caps
containing disinfecting agent
(IPA) have been shown to
reduce intraluminal microbial
contamination and reduce rates
of CLABSIs.11” (Level II)



3M™ Curoso™
Disinfecting Cap for
Needleless Connectors



3M™ Curoso™ Tips™
Disinfecting Cap
For Male-Luers



3M™ Curoso™
Disinfecting Cap for Tego®
Hemodialysis Connectors



3M™ Curoso™ Stopper
Disinfecting Cap for
Open Female Luers

Where you need them, when you need them.

Curos products can be dispensed as individual caps or on strips. Strips of Curos products can be hung from I.V. poles for easy access, greater compliance and reduced waste.

Powerful 1 minute disinfection

Curos disinfecting port protectors contain 70% isopropyl alcohol (IPA). The IPA disinfects the surface of the port in 1 minute. They're proven effective disinfecting against *Staphylococcus aureus*, *Staphylococcus epidermidis*, *Escherichia coli*, *Pseudomonas aeruginosa*, *Candida glabrata*, and *Candida albicans*^{7,8}.

Protects for up to 7 days

Curos disinfecting port protectors can also be left in place to keep ports clean and protected for up to 7 days. Passive disinfection removes human technique variance, providing consistent disinfection every time.

Colored bright to disinfect right

Brightly colored Curos products verify that a port is clean at a glance and disinfection compliance can be easily and reliably measured.

Protection that stays put

Curos disinfecting port protectors twist on easily and stay securely in place on commonly used ports — meeting INS guidelines for add-on devices.



Strips are consistent with the INS Guideline:

“Ensure disinfecting supplies are readily available at bedside to facilitate staff compliance with port disinfection.”¹¹

¹¹ Gorski L, Hadaway L, Hagle ME, McGoldrick M, Orr M, Doellman D. Infusion Therapy Standards of Practice. Journal of Infusion Nursing. 2016; 39(suppl 1):S1-S159.



Peer-reviewed articles

Clinical studies back us up

Several hospitals have implemented the use of Curos disinfecting caps and achieved impressive results.

10% increase in nurse compliance resulted in a statistically significant

7%
decrease in
infection rates

Implementation of the strip version of Curos caps during the trial increased compliance rates from

63% to 80%

American Journal of Infection Control: Volume 40 Number 12; December 2014

Impact of Universal Disinfectant Cap Implementation on Central Line-Associated Bloodstream Infections

Katreena Collette Merrill RN, PhD, Sharon Sumner RN, BS, Lorraine Linford RN, BS, CNSC, Carrie Taylor RN, MS, CIC, Christopher Macintosh RN, BS.

- The rate of CLABSI infections decreased by >40% following implementation of the 3M™ Curos™ Disinfecting Strip for Needleless Connectors (IRR = .557, P = .004).
- Curos Cap use was associated with an estimated savings of almost \$300,000 per year in the hospital studied.
- Weekly audits of compliance demonstrated that a 10% increase in nurse compliance resulted in a statistically significant 7% drop in infection rate.

The Journal of the Association for Vascular Access: Volume 17 Number 4; December 2012

Central Venous Catheter Protective Connector Caps Reduce Intraluminal Catheter-Related Infection

Chuck Ramirez, BA, RRT, VA-BC, Antonina M. Lee, MEd, MPH, RN, CIC, Ken Welch, MD
Banner Estrella Medical Center, Phoenix, AZ

- During 2010, the CLABSI rate reduced from 1.9 in 2010 to 0.5 during the one-year trial period.
- The implementation of 3M™ Curos™ Disinfecting Strip for Needleless Connectors during month five of the trial increased compliance rates from 63% to 80%.

This infection reduction could translate to an annual savings of approximately

\$3.7 million

32-bed study showed annual savings of

\$500,000

Curo caps were estimated to provide a potential clinical time saving of

82.4
working days
per year

American Journal of Critical Care, Vol. 25, No. 2: 165-172, March 2016

Use of a Central Catheter Maintenance Bundle in Long-term Care Hospitals

Anthony M. Grigonis, PhD, Amanda M. Dawson, PhD, Mary Burkett, DNP, CNS, Arthur Dylag, MA, MBA, Matthew Sears, BS, Betty Helber, RN, MS, ANE-BC, and Lisa K. Snyder, MN, MPH

- A central catheter maintenance bundle was implemented in 30 LTACHs, and compliance with the bundle was tracked for six months. CLABSI rates were monitored for 14 months before and 14 months after the bundle was implemented.
- In addition to the CDC guidelines, the bundle protocol included education on the protocol, mandatory use of alcohol-based central catheter caps, chlorhexidine gluconate dressings, and formation of a central catheter team of nurses.
- A mean reduction of 4.5 CLABSIs per LTACH occurred for the LTACHs studied for 14 months after the bundle was implemented. This infection reduction could translate to a savings of approximately \$3.7 million annually for the 30 LTACHs studied and could have potentially saved 20 patients' lives, assuming a 15% mortality rate from CLABSIs.

American Journal of Infection Control: Volume 40 Number 10; December 2012

Impact of Alcohol Impregnated Port Protectors and Needleless Neutral Pressure Connectors on Central Line-Associated Bloodstream Infections and Contamination of Blood Cultures in an Inpatient Oncology Unit

Michael A. Sweet, PharmD; Aaron Cumpston, PharmD; Frank Briggs, PharmD; MPH, Michael Craig MD and Mehdi Hamadani, MD

- A total of 6,851 central line-days and 16 CLABSIs (2.3 infections/1,000 central line days) were documented during the control period, compared with 3,005 central line days and one CLABSI (a rate of 0.3 infections/1,000 central line days) during the intervention period (relative risk, 0.14; 95% confidence interval [CI], 0.02-1.07; P = .03).
- This 32-bed study showed \$500,000 in annualized savings (Sweet MA, et al. SHEA Product Evaluation 2011).
- The rate of contaminated blood cultures from central lines was 2.5% (17 of 692) during the control period, but only 0.2% (1 of 470) during the intervention period (relative risk, 0.09; 95% CI, 0.01-0.65; P = .002).
- The rate of adherence to the intervention was 85.2% (228 of 269 patients with catheter protectors).

British Journal of Nursing: (IV Therapy Supplement) Vol 25, No 8, 2016

Port Protectors in Clinical Practice: an Audit

Corinne Cameron-Watson. Barking Havering and RedBridge NHS Trust

- The study measured the effect on compliance and incidence of vascular access device (VAD)-related bacteremia following the introduction of a passive disinfection device (Curo) for 6 months.
- As compared to data collected in a benchmark "scrub the hub" audit, data post Curo cap implementation showed VAD-related bacteremia rates reduced by 69% when staff compliance with Curo cap placement onto VADs was 80% or more.
- The use of Curo caps was estimated to provide a potential clinical-time saving of 659.4 hours per year, which equates to 82.4 working days per year (based on an 8-hour day).
- Of the 86 staff trained to use a port protector, 70% returned completed questionnaire, and of these 100% preferred the port protectors to manual scrubbing.

The entire family of 3M™ Curoso™ Disinfecting Port Protectors

Disinfects in 1 minute

Protects ports for up to 7 days

Twists on, stays on

Brightly colored for visual
verification and auditing

Single use only



3M™ Curoso™

Disinfecting Cap for Needleless
Connectors

Disinfects

Disinfects needleless connectors
in 1 minute.

Protects


Acts as a barrier to contamination while
in place.

Where you need them, when you need them

Strips of Curoso products can be hung
from I.V. poles for easy access, greater
compliance and reduced waste.

Dispensing options

- Individual caps
- Strips (10 count)

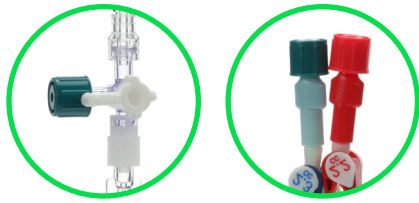

3M™ Curostopper™

Disinfecting Cap for Open Female Luers

Thoughtful design

Curostopper disinfecting caps are designed to luer lock onto a wide range of stopcocks and catheter hubs. They utilize 70% isopropyl alcohol (IPA) to disinfect the critical surfaces of open female luers, prior to line access.

The unique cap design will hold pressure to maintain a closed system.

Dispensing options

- Individual caps
- Strips (5 count)



3M™ Curocaps™

Disinfecting Cap for Tego® Hemodialysis Connectors

Compatible

This specially designed Curocaps disinfecting cap has been tested to fit and maintain the integrity of the Tego® Hemodialysis Connector.

*ICU Medical. "Tego Swab Recommendations and Compatibility with Disinfecting Caps," October, 2012.

Custom colored

White Curocaps for Tego hemodialysis connectors are easily distinguished from green caps for dedicated use on the Tego connectors.

Dispensing options

- Individual caps



3M™ Curocaps™ Tips

Disinfecting Cap for Male Luers

Protection where it's needed

Curocaps Tips disinfecting caps contain 70% IPA within their inner cavity to disinfect and protect the distal end of I.V. tubing and other male luer devices.

Optimal alcohol placement

A unique design shields excess alcohol from entering while providing sufficient flow of alcohol precisely where it is needed — on the exposed exterior male luer.

Dispensing options

- Strips (5 count)

Need help incorporating Curos products into your hospital processes?



We want everyone who uses Curos products to be successful. We offer the services of a Clinical Outcomes Team that can help hospitals implement the use of Curos products to achieve and sustain high compliance. Our team consists of full-time nurses dedicated to supporting your efforts.

Areas we can assist with:

- Planning resources and guidance.
- Sharing proprietary processes and tools that spur adoption and measure your success.
- Implementation and large trial support.
- Compliance tools for training, motivating and auditing.
- On-going consulting and support.
- Assistance in study creation and results reporting.
- Point prevalence reviews to help you reduce risk at all access points.
- Clinical expertise regarding standards, guidelines, and how 3M products can help you achieve successful outcomes.



Continuing Education

Our Healthcare Academy is an online site that contains over 50 free CE credit courses.

For more information visit:
www.3M.com/learningconnection

Try our other antimicrobial protection products

We offer a range of vascular care products to help you achieve better patient outcomes. For more information, visit 3M.com/IVcare

To order call:
800-228-3957

To learn more about how Solvetum can help you and your facility protect clinician and patient safety, prevent costly I.V. site complications, and improve patient satisfaction, contact your 3M Critical & Chronic Care Solutions representative or call the Solvetum Health Care Customer Helpline at 1-800-228-3957. Outside of the United States, contact the local Solvetum subsidiary.

For more information, go to 3M.com/C3SD

Product	Dispenser	Product order #	Boxes per case	Units per box	Total caps or tips per case
3M™ Curos™ Disinfecting Caps for Needleless Connectors	Individuals	CFF1-270R	10	270	2,700
	Strips (10 count)	CFF10-250R	10	25 Strips	2,500
3M™ Curos Tips™ Disinfecting Caps for Male Luers	Strips (5 count)	CM5-200R	10	40 Strips	2,000
3M™ Curos™ Disinfecting Caps for Tego® Hemodialysis Connectors	Individuals	CTG1-270R	8	270	2,160
3M™ Curos™ Stopper Disinfecting Caps for Open Female Luers	Individuals – Teal	CSV1-270R	8	270	2,160
	Strips – Teal (5 count)	CSV5-250R	8	50 Strips	2,000
	Individuals – Red	CSA1-270R	8	270	2,160
	Strips – Red (5 count)	CSA5-250R	8	50 Strips	2,000

Solvetum Medical Surgical

Phone 800-228-3957
 Web Go.Solvetum.com/Curos

© Solvetum 2026. Solvetum and the S logo are trademarks of Solvetum or its affiliates. 3M, the 3M logo and other 3M owned and/or licensed trademarks are trademarks of 3M. Other trademarks are the property of their respective owners.

70-2011-6861-7