




Attest™

Sterilization Solutions


3M Sterilization Assurance

Easy-to-Read 3M™ Attest™ Steam Chemical Integrators, Type 5


Unprocessed

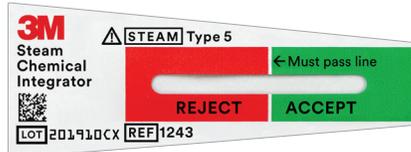

Processed

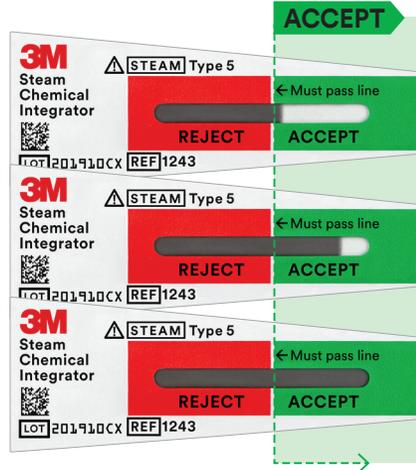

Processed

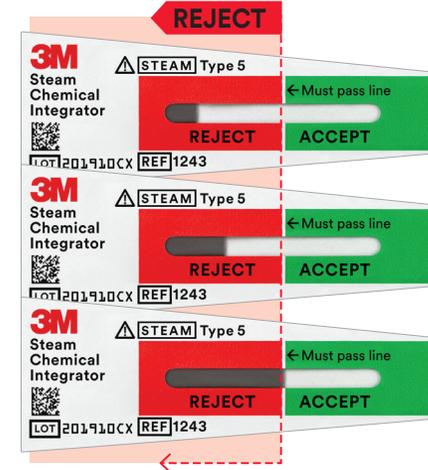

3M™ Attest™ Steam Chemical Integrators, Type 5 comply with ISO 11140-1:2014.

© 2020 3M. All rights reserved. 3M and Attest are marks and/or registered marks of 3M. Unauthorized use prohibited. Used under license in Canada.

70-2009-8636-5

The color bar has reached the **ACCEPT** window in all three samples shown above, indicating that the necessary conditions for sterilization have been met. **If the color bar crosses into the ACCEPT region, it is considered a pass.**

The color bar is in the **REJECT** window, indicating that the necessary conditions for sterilization have not been met. The pack should be reprocessed and the cause of sterilization failure should be investigated. **If the color bar is in the REJECT region or on the line, it is considered a fail.**