

3M™ Tube Securement Device


This strong, easy-to-use solution secures non-critical medical tubes made from silicone, PVC and silicone coated latex. It is gentle to skin and designed to support pressure injury and medical adhesive-related skin injury (MARSI) prevention practices.

Uniquely shaped

Designed to lift tubes off skin and help promote consistent application.

Sterile device

In single-use packaging.

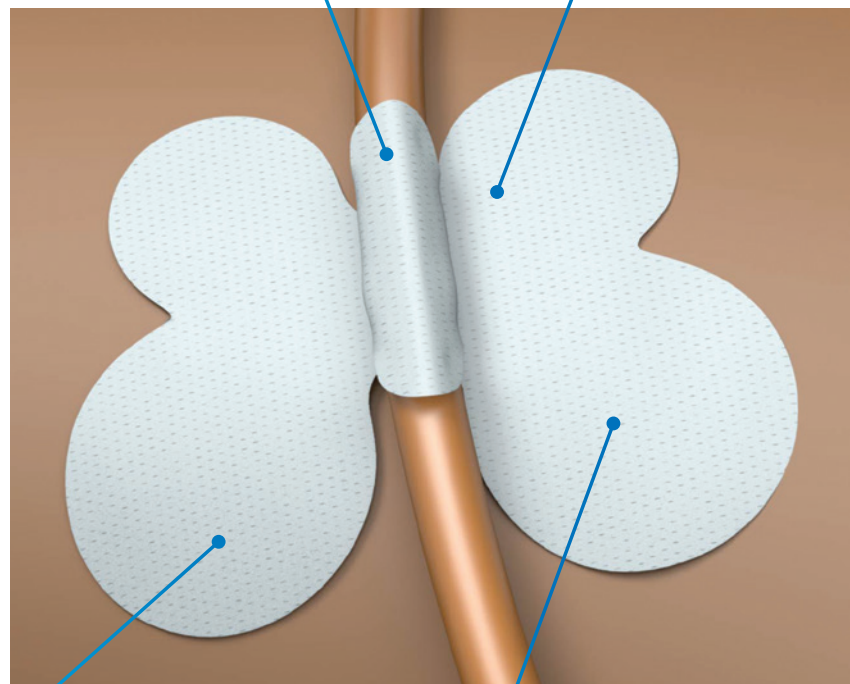

Reinforced soft cloth backing

Provides extra strength and flexibility.

Two sizes

Small device for medical tubes and catheters 6–12 Fr and large device for medical tubes and catheters 12–24 Fr.



Skin performance: The feather designates products that deliver the securement power you need while minimising damage to skin.

Reliable securement

Unique adhesive secures medical tubes and catheters for up to 4 days.¹

Ease of use

Easy to apply and removes cleanly in one piece; allows for standardisation of technique.

Gentle to skin

Non-sensitising silicone adhesive has low potential to cause dermatitis with minimal skin damage and pain upon removal.¹

Designed to help reduce pressure injury risk

With no hard components to cause pressure, product's unique shape minimises contact between skin and tube.


When it comes to tube securement selection there are a variety of factors to keep in mind, including securement performance, skin protection and clinician ease of use. Consider the results of comparative studies, such as the one below, to help inform your decision.

A comparison of the 3M™ Tube Securement Device to the StatLock® Foley Stabilisation Device.¹

Wear time

Dependability and length of wear are important in choosing the right device.


The 3M™ Tube Securement Device had a statistically higher percentage of devices with the tube in place after a 72 hour wear than StatLock® Foley Stabilisation Device.*

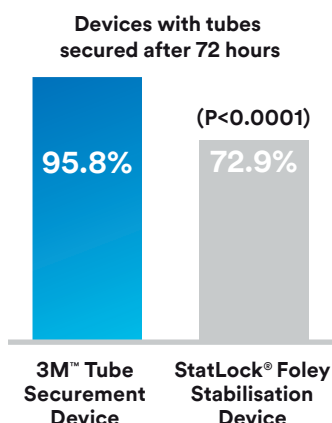

Skin integrity

Skin is the body's first line of defense, so it is important to protect it.


Consider this comparison of the impact on the skin's barrier function (measured by average change in Transepidermal Water Loss (TEWL) from pre-treatment).

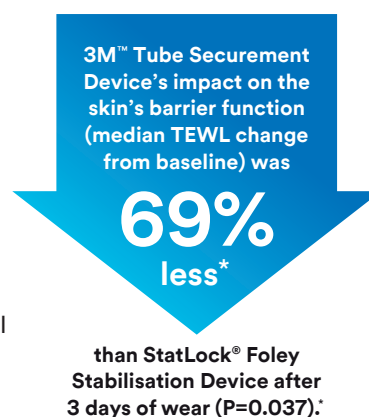

Removal time

Efficient removal is critical when clinician time is limited.

The average removal time for 3M™ Tube Securement Device was 13 seconds compared to 126 seconds for StatLock® Foley Stabilisation Device (P<0.0001).

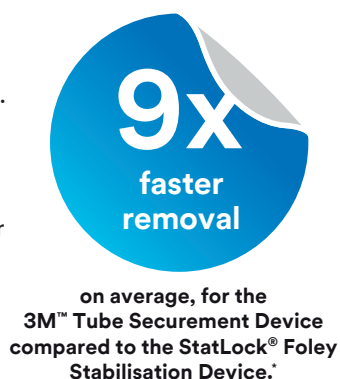


Wipes for removal

Extra supplies can add time and cost to a procedure.

On average, the StatLock® Foley Stabilisation Device required 12 alcohol wipes for removal, while the 3M™ Tube Securement Device does not require a removal agent.*

Average number of wipes used for removal

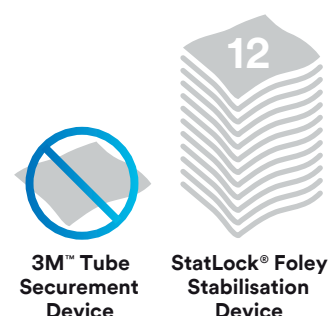

Feel secure in your choice. Trust the science behind 3M™ Tube Securement Device for reliable performance.

To order, contact your 3M Health Care Sales Representative or call the 3M Health Care Customer Helpline at 08705 360036. Visit 3M.co.uk/Medical for more information.

Refer to product Instructions for Use (IFU) for other important information.

Ordering information

Product	Product name	Product number	Size	Devices/box	Boxes/case
	3M™ Tube Securement Device, Large	1501U	5.5cm x 9.0cm	25	4
	3M™ Tube Securement Device, Small	1500U	4.3cm x 6.1cm	25	4

Medical Care Solutions Division

3M United Kingdom PLC
Charnwood Campus
10 Bakewell Road
Loughborough
LE11 5RB
+44 (0)1509 611 611

3M Ireland
The Iveagh Building
Carrickmines Park
Carrickmines
Dublin 18
00 353 (01) 280 3555

*As tested in a comparative, prospective clinical study on 24 healthy human subjects after 3 days of wear followed by device removal from skin per IFU.

© 2022 3M. All rights reserved. 3M and the other marks shown are marks and/or registered marks. Unauthorised use prohibited All other marks are property of their respective owners. All rights reserved. OMG359355. GF755.

